

# Summary Report of IQC program for G6PD Quantitative Test - AMP Group - March 2017 -


## I. The statistic results of all laboratories in this month

G6PD	Control N (Lot No.:AC1203N)	Control D (Lot No.:AC1203D)
Labs	8	8
Received results number (n)	40	40
Median	11.9 (U/gHb)	2.8 (U/gHb)
Mean	11.7 (U/gHb)	2.8 (U/gHb)
SD	1.0	0.3
CV	8.5%	10.7%
Range of G6PD	9.9 ~ 14.1 (U/gHb)	2.2 ~ 3.4 (U/gHb)
Range of Hb	2.0 ~ 2.9 (g/dL)	2.3 ~ 3.6 (g/dL)

\*The statistic results are calculated from all labs reported in this month

\*\* G6PD Method = AMP reagent kit, 37°C

## II. The distribution of G6PD reported for each lab in this survey

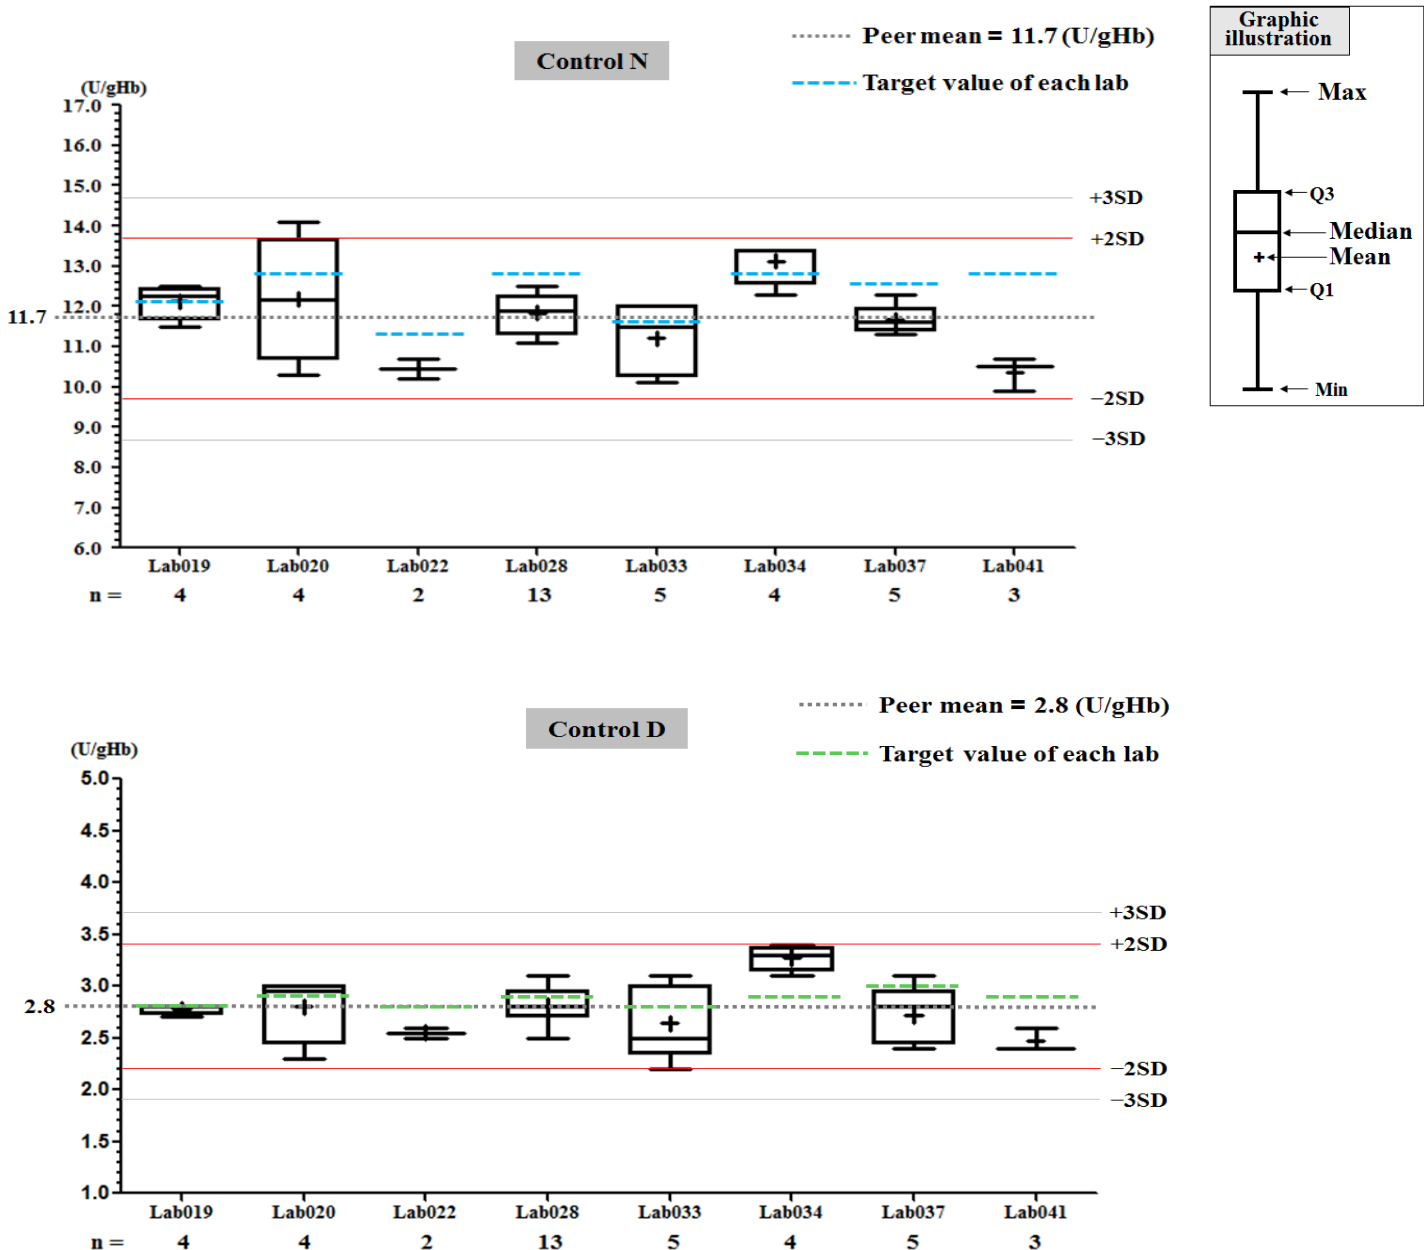

# QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AC1203N (2014-01-01 ~ 2100-12-31) [Change](#)

[Print Table](#)

## Lab033

QC Control Lot No.	Control N		Control D	
	AC1203N		AC1203D	
Duration of the Analyzing	Month (2017/03)	CUM (2016/10/13~2017/03/31)	Month (2017/03)	CUM (2016/10/13~2017/03/31)
Runs (N)	5	26	5	26
Mean (U/gHb)	11.2	11.6	2.6	2.8
SD	0.9	0.9	0.4	0.3
CV (%)	8.0	7.8	15.4	10.7
Target Value (U/gHb)	11.6	11.6	2.8	2.8
Total Error (%)	19.5	15.5	37.9	21.4
TEa (%)	20	20	20	20
$\sigma$	2.1	2.6	0.8	1.9

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 $\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)


Month : 2017 | 03 [Change](#) ; Cumulative : from 2016 | 10 | 13 to 2017 | 03 | 31 [Change](#)

[TOP](#)

## Control N SDI QC Chart

Lot No.: AC1203N ; Duration : 2016-10-13 to 2017-03-31 ; Target : 11.6 ; SD : 1.20

Lab033

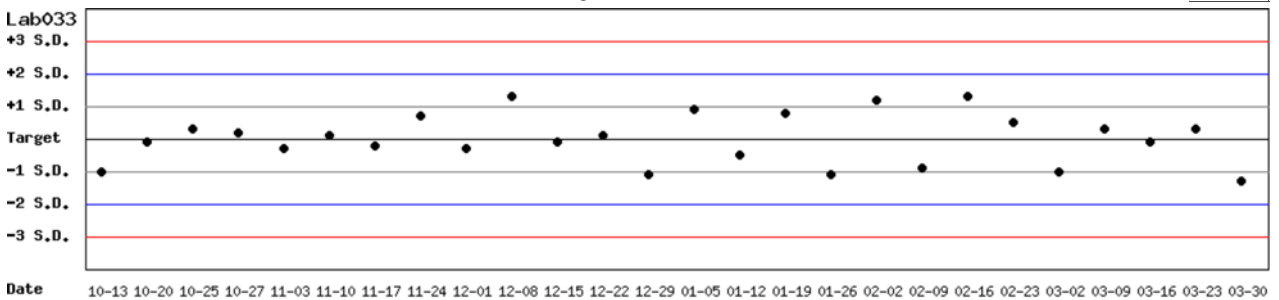


Month : 2017 | 03 [Change](#) ; Cumulative : from 2016 | 10 | 13 to 2017 | 03 | 31 [Change](#)

[TOP](#)

## Control D SDI QC Chart

Lot No.: AC1203D ; Duration : 2016-10-13 to 2017-03-31 ; Target : 2.8 ; SD : 0.30

Lab033

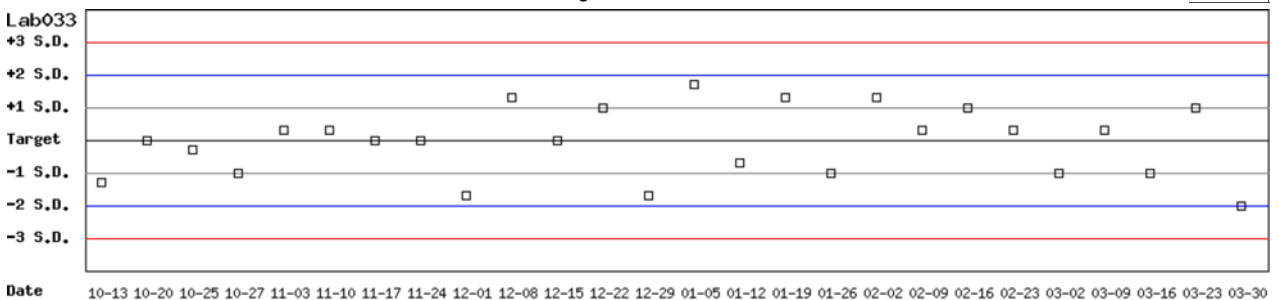

Month : 2017 | 03 [Change](#) ; Cumulative : from 2016 | 10 | 13 to 2017 | 03 | 31 [Change](#)


[TOP](#)

## Control N and Control D SDI QC Chart

Lot No.: AC1203N ; Duration : 2016-10-13 to 2017-03-31 ; Target : 11.6 ; SD : 1.20 ( ● )

Lot No.: AC1203D ; Duration : 2016-10-13 to 2017-03-31 ; Target : 2.8 ; SD : 0.30 ( □ )

Lab033

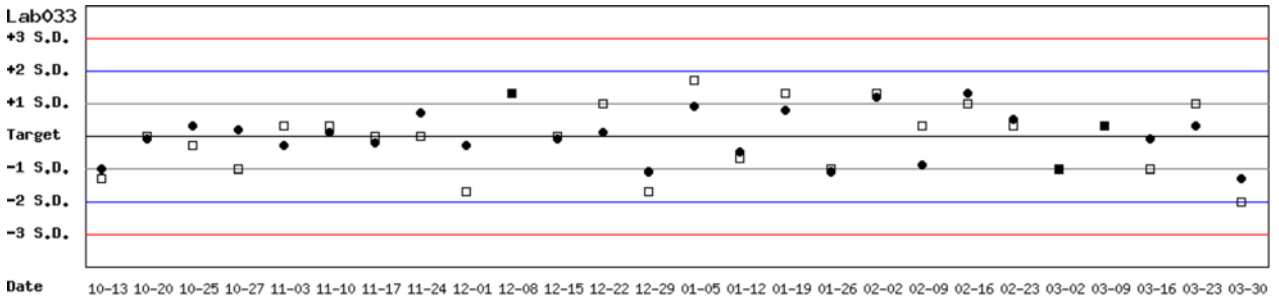

Month : 2017 | 03 | Change ; Cumulative : from 2016 | 10 | 13 to 2017 | 03 | 31 | Change

[\[TOP\]](#)

## Peer Group Statistics (Table 1)

Select LotNo : AC1203N (2014-01-01 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 2 - AMP ▼ Change

[Print Table 1](#)

### Monthly

Month : 2017 ▼ 03 ▼ Change

UnitID <sup>↑</sup>	Reagent Kit (Code) <sup>↑</sup>	Control N (Lot No.: AC1203N)									Control D (Lot No.: AC1203D)						
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab019</a>	2	12.1	12.1	4	0.4	3.3	6.6	20	>6	2.8	2.8	4	0.1	3.6	7.1	20	5.6
<a href="#">Lab020</a>	2	12.8	12.2	4	1.6	13.1	30.9	20	1.2	2.9	2.8	4	0.3	10.7	24.9	20	1.5
<a href="#">Lab022</a>	2	11.3	10.5	2	-	-	-	20	-	2.8	2.6	2	-	-	-	20	-
<a href="#">Lab028</a>	2	12.8	11.8	13	0.5	4.2	16.3	20	2.9	2.9	2.8	13	0.2	7.1	17.7	20	2.3
<a href="#">Lab033</a>	2	11.6	11.2	5	0.9	8.0	19.5	20	2.1	2.8	2.6	5	0.4	15.4	37.9	20	0.8
<a href="#">Lab034</a>	2	12.8	13.1	4	0.6	4.6	11.5	20	3.8	2.9	3.3	4	0.1	3.0	19.9	20	2.1
<a href="#">Lab037</a>	2	12.6	11.7	5	0.4	3.4	14.0	20	3.8	3.0	2.7	5	0.3	11.1	32.2	20	0.9
<a href="#">Lab041</a>	2	12.8	10.4	3	0.4	3.8	26.4	20	0.3	2.9	2.5	3	0.1	4.0	21.8	20	1.6
Total	-	-	11.7	40	1.0	8.5	-	-	-	-	2.8	40	0.3	10.7	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

### Cumulative

Cumulative : from 2014 ▼ 02 ▼ 01 ▼ to 2017 ▼ 03 ▼ 31 ▼ Change

UnitID <sup>↑</sup>	Reagent Kit (Code) <sup>↑</sup>	Control N (Lot No.: AC1203N)									Control D (Lot No.: AC1203D)						
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab017</a>	2	14.2	13.8	36	1.6	11.6	26.0	20	1.5	3.3	3.9	36	1.4	35.9	90.0	20	0.1
<a href="#">Lab018</a>	2	10.9	10.9	113	1.3	11.9	23.9	20	1.7	2.5	2.6	113	0.9	34.6	73.2	20	0.5
<a href="#">Lab019</a>	2	12.1	12.2	157	1.1	9.0	18.9	20	2.1	2.8	2.8	157	0.4	14.3	28.6	20	1.4
<a href="#">Lab020</a>	2	12.8	11.8	19	1.4	11.9	31.5	20	1.0	2.9	2.7	19	0.5	18.5	43.9	20	0.7
<a href="#">Lab021</a>	2	12.3	13.5	88	1.0	7.4	24.6	20	1.4	2.8	3.2	88	0.3	9.4	33.0	20	0.6
<a href="#">Lab022</a>	2	11.3	11.5	65	1.2	10.4	22.6	20	1.8	2.8	2.9	65	0.3	10.3	24.3	20	1.6
<a href="#">Lab024</a>	2	11.6	11.1	58	1.2	10.8	25.9	20	1.5	2.7	2.7	58	0.3	11.1	22.2	20	1.8
<a href="#">Lab026</a>	2	11.6	11.5	212	1.6	13.9	28.7	36	2.5	2.7	2.8	212	0.5	17.9	39.4	36	1.8
<a href="#">Lab027</a>	2	12.3	11.8	151	1.6	13.6	31.2	20	1.2	2.9	2.7	151	0.5	18.5	43.9	20	0.7
<a href="#">Lab028</a>	2	12.8	13.5	338	1.2	8.9	23.2	20	1.6	2.9	3.3	338	0.5	15.2	44.1	20	0.4
<a href="#">Lab031</a>	2	12.8	10.4	89	1.5	14.4	47.6	20	0.1	2.9	2.5	89	0.5	20.0	53.8	20	0.3
<a href="#">Lab032</a>	2	12.3	11.5	222	1.9	16.5	39.5	20	0.8	2.9	2.7	222	0.5	18.5	43.9	20	0.7
<a href="#">Lab033</a>	2	11.6	11.9	152	1.0	8.4	19.4	20	2.1	2.8	2.9	152	0.3	10.3	24.3	20	1.6
<a href="#">Lab034</a>	2	12.8	12.3	90	0.7	5.7	15.3	20	2.8	2.9	3.0	90	0.3	10.0	23.4	20	1.7
<a href="#">Lab035</a>	2	12.8	12.4	55	0.7	5.6	14.4	20	3.0	2.9	2.8	55	0.3	10.7	24.9	20	1.5
<a href="#">Lab037</a>	2	12.6	12.2	66	1.2	9.8	22.8	20	1.7	3.0	2.9	66	0.4	13.8	30.9	20	1.2
<a href="#">Lab038</a>	2	12.8	12.7	60	1.0	7.9	16.5	20	2.4	2.9	3.2	60	0.5	15.6	41.6	20	0.6
<a href="#">Lab040</a>	2	12.8	12.1	21	0.5	4.1	13.7	20	3.5	2.9	2.6	21	0.3	11.5	33.4	20	0.8
<a href="#">Lab041</a>	2	12.8	10.4	4	0.4	3.8	26.4	20	0.3	2.9	2.5	4	0.1	4.0	21.8	20	1.6
Total	-	-	12.1	1996	1.6	13.2	-	-	-	-	2.9	1996	0.6	20.7	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

Reagent Kit	Reagent Code
AMP	2

## Peer Group Statistics (Table 2)

Select LotNo : AC1203N (2014-01-01 ~ 2100-12-31) Change

Select Reagent Kit : 2 - AMP Change

[Print Table 2](#)

### Control N Month vs. Cumulative

Control N (Lot No.: AC1203N)																	
UnitID <sup>†</sup>	Reagent Kit (Code) <sup>‡</sup>	Month (2017/03)									CUM (2014/02/01~2017/03/31)						
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab017</a>	2	14.2	-	0	-	-	-	20	-	14.2	13.8	36	1.6	11.6	26.0	20	1.5
<a href="#">Lab018</a>	2	10.9	-	0	-	-	-	20	-	10.9	10.9	113	1.3	11.9	23.9	20	1.7
<a href="#">Lab019</a>	2	12.1	12.1	4	0.4	3.3	6.6	20	>6	12.1	12.2	157	1.1	9.0	18.9	20	2.1
<a href="#">Lab020</a>	2	12.8	12.2	4	1.6	13.1	30.9	20	1.2	12.8	11.8	19	1.4	11.9	31.5	20	1.0
<a href="#">Lab021</a>	2	12.3	-	0	-	-	-	20	-	12.3	13.5	88	1.0	7.4	24.6	20	1.4
<a href="#">Lab022</a>	2	11.3	10.5	2	-	-	-	20	-	11.3	11.5	65	1.2	10.4	22.6	20	1.8
<a href="#">Lab024</a>	2	11.6	-	0	-	-	-	20	-	11.6	11.1	58	1.2	10.8	25.9	20	1.5
<a href="#">Lab026</a>	2	11.6	-	0	-	-	-	36	-	11.6	11.5	212	1.6	13.9	28.7	36	2.5
<a href="#">Lab027</a>	2	12.3	-	0	-	-	-	20	-	12.3	11.8	151	1.6	13.6	31.2	20	1.2
<a href="#">Lab028</a>	2	12.8	11.8	13	0.5	4.2	16.3	20	2.9	12.8	13.5	338	1.2	8.9	23.2	20	1.6
<a href="#">Lab031</a>	2	12.8	-	0	-	-	-	20	-	12.8	10.4	89	1.5	14.4	47.6	20	0.1
<a href="#">Lab032</a>	2	12.3	-	0	-	-	-	20	-	12.3	11.5	222	1.9	16.5	39.5	20	0.8
<a href="#">Lab033</a>	2	11.6	11.2	5	0.9	8.0	19.5	20	2.1	11.6	11.9	152	1.0	8.4	19.4	20	2.1
<a href="#">Lab034</a>	2	12.8	13.1	4	0.6	4.6	11.5	20	3.8	12.8	12.3	90	0.7	5.7	15.3	20	2.8
<a href="#">Lab035</a>	2	12.8	-	0	-	-	-	20	-	12.8	12.4	55	0.7	5.6	14.4	20	3.0
<a href="#">Lab037</a>	2	12.6	11.7	5	0.4	3.4	14.0	20	3.8	12.6	12.2	66	1.2	9.8	22.8	20	1.7
<a href="#">Lab038</a>	2	12.8	-	0	-	-	-	20	-	12.8	12.7	60	1.0	7.9	16.5	20	2.4
<a href="#">Lab040</a>	2	12.8	-	0	-	-	-	20	-	12.8	12.1	21	0.5	4.1	13.7	20	3.5
<a href="#">Lab041</a>	2	12.8	10.4	3	0.4	3.8	26.4	20	0.3	12.8	10.4	4	0.4	3.8	26.4	20	0.3
Total	-	-	11.7	40	1.0	8.5	-	-	-	-	12.1	1996	1.6	13.2	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2017 03 Change

Cumulative : from 2014 02 01 to 2017 03 31 Change

[TOP](#)

### Control D Month vs. Cumulative

Control D (Lot No.: AC1203D)																	
UnitID <sup>†</sup>	Reagent Kit (Code) <sup>‡</sup>	Month (2017/03)									CUM (2014/02/01~2017/03/31)						
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab017</a>	2	3.3	-	0	-	-	-	20	-	3.3	3.9	36	1.4	35.9	90.0	20	0.1
<a href="#">Lab018</a>	2	2.5	-	0	-	-	-	20	-	2.5	2.6	113	0.9	34.6	73.2	20	0.5
<a href="#">Lab019</a>	2	2.8	2.8	4	0.1	3.6	7.1	20	5.6	2.8	2.8	157	0.4	14.3	28.6	20	1.4
<a href="#">Lab020</a>	2	2.9	2.8	4	0.3	10.7	24.9	20	1.5	2.9	2.7	19	0.5	18.5	43.9	20	0.7
<a href="#">Lab021</a>	2	2.8	-	0	-	-	-	20	-	2.8	3.2	88	0.3	9.4	33.0	20	0.6
<a href="#">Lab022</a>	2	2.8	2.6	2	-	-	-	20	-	2.8	2.9	65	0.3	10.3	24.3	20	1.6
<a href="#">Lab024</a>	2	2.7	-	0	-	-	-	20	-	2.7	2.7	58	0.3	11.1	22.2	20	1.8
<a href="#">Lab026</a>	2	2.7	-	0	-	-	-	36	-	2.7	2.8	212	0.5	17.9	39.4	36	1.8
<a href="#">Lab027</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.7	151	0.5	18.5	43.9	20	0.7
<a href="#">Lab028</a>	2	2.9	2.8	13	0.2	7.1	17.7	20	2.3	2.9	3.3	338	0.5	15.2	44.1	20	0.4
<a href="#">Lab031</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.5	89	0.5	20.0	53.8	20	0.3
<a href="#">Lab032</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.7	222	0.5	18.5	43.9	20	0.7
<a href="#">Lab033</a>	2	2.8	2.6	5	0.4	15.4	37.9	20	0.8	2.8	2.9	152	0.3	10.3	24.3	20	1.6
<a href="#">Lab034</a>	2	2.9	3.3	4	0.1	3.0	19.9	20	2.1	2.9	3.0	90	0.3	10.0	23.4	20	1.7
<a href="#">Lab035</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.8	55	0.3	10.7	24.9	20	1.5
<a href="#">Lab037</a>	2	3.0	2.7	5	0.3	11.1	32.2	20	0.9	3.0	2.9	66	0.4	13.8	30.9	20	1.2
<a href="#">Lab038</a>	2	2.9	-	0	-	-	-	20	-	2.9	3.2	60	0.5	15.6	41.6	20	0.6
<a href="#">Lab040</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.6	21	0.3	11.5	33.4	20	0.8
<a href="#">Lab041</a>	2	2.9	2.5	3	0.1	4.0	21.8	20	1.6	2.9	2.5	4	0.1	4.0	21.8	20	1.6
Total	-	-	2.8	40	0.3	10.7	-	-	-	-	2.9	1996	0.6	20.7	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2017 03 Change

Cumulative : from 2014 02 01 to 2017 03 31 Change

[TOP](#)

Reagent Kit	Reagent Code
AMP	2