

# QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AE0909N (2016-01-01 ~ 2100-12-31) [Change](#)

[Print Table](#)

## Lab040

QC Control Lot No.	Control N		Control D	
	Month (2020/07)	CUM (2018/04/26~2020/07/31)	Month (2020/07)	CUM (2018/04/26~2020/07/31)
Duration of the Analyzing	1	26	1	26
Runs (N)	12.8	13.6	4.5	4.8
Mean (U/gHb)	-	0.5	-	0.3
SD	-	3.7	-	6.3
CV (%)	14.4	14.4	5.8	5.8
Target Value (U/gHb)	-	12.9	-	29.7
Total Error (%)	20	20	20	20
TEa (%)	-	3.9	-	0.4
$\sigma$	-		-	

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 x CV (%)

$\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2020 07 [Change](#) ; Cumulative : from 2018 04 26 to 2020 07 31 [Change](#)


[TOP](#)

## Control N and Control D SDI QC Chart

Lot No.: AE0909N ; Duration : 2018-04-26 to 2020-07-31 ; Target : 14.4 ; SD : 0.6 (●)

Lot No.: AE0909D ; Duration : 2018-04-26 to 2020-07-31 ; Target : 5.8 ; SD : 0.3 (□)

Lab040

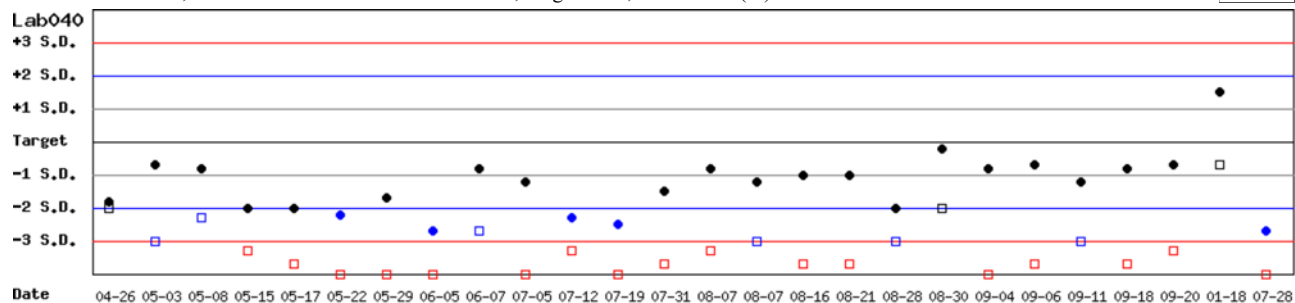


Month : 2020 07 [Change](#) ; Cumulative : from 2018 04 26 to 2020 07 31 [Change](#)

[TOP](#)

## Control N SDI QC Chart

Lot No.: AE0909N ; Duration : 2018-04-26 to 2020-07-31 ; Target : 14.4 ; SD : 0.6

Lab040

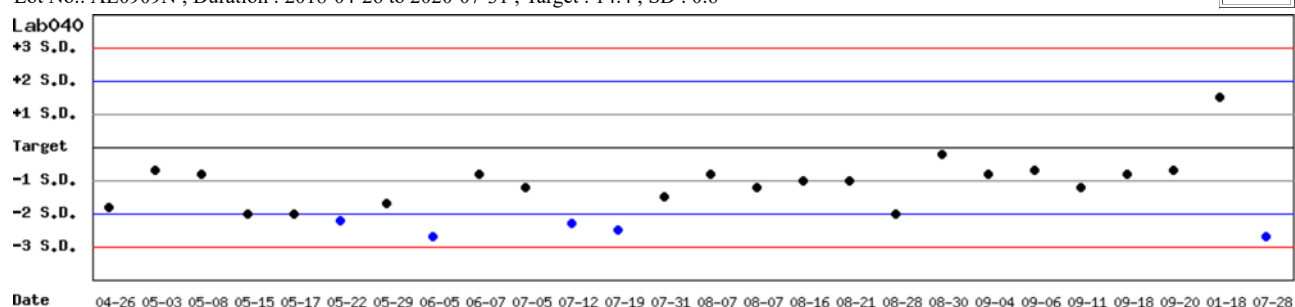


Month : 2020 07 [Change](#) ; Cumulative : from 2018 04 26 to 2020 07 31 [Change](#)

[TOP](#)

## Control D SDI QC Chart

Lot No.: AE0909D ; Duration : 2018-04-26 to 2020-07-31 ; Target : 5.8 ; SD : 0.3

Lab040

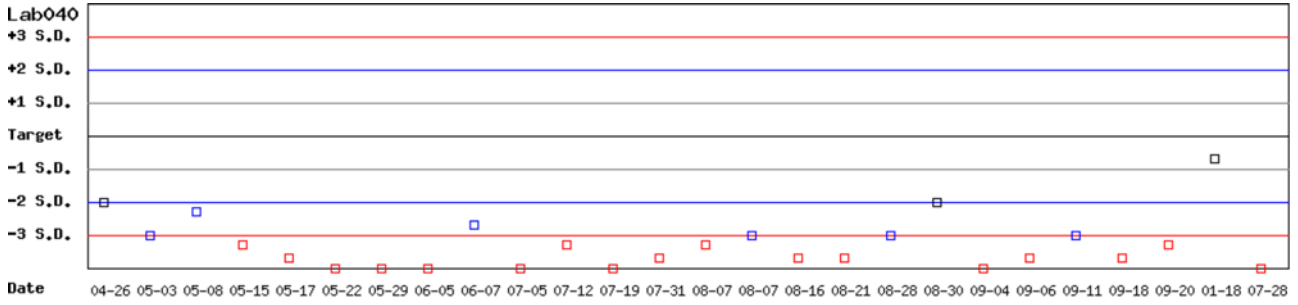

Month : 2020 | 07 | Change ; Cumulative : from 2018 | 04 | 26 | to 2020 | 07 | 31 | Change

[\[TOP\]](#)

# Peer Group Statistics (Table 1)

Select LotNo : AE0909N (2016-01-01 ~ 2100-12-31)

Select Reagent Kit : 5 - Medicon

## Monthly

Month : 2020  07

		Control N (Lot No.: AE0909N)								Control D (Lot No.: AE0909D)							
UnitID <input type="button" value="↑"/>	Reagent Kit (Code) <input type="button" value="↑"/>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab019</a>	5	15.3	14.9	1	-	-	-	20	-	5.3	4.8	1	-	-	-	20	-
<a href="#">Lab026</a>	5	15.9	12.9	17	0.1	0.8	20.4	20	1.4	5.8	4.9	17	0.2	4.1	23.7	20	1.1
<a href="#">Lab034</a>	5	15.5	15.5	5	0.8	5.2	10.3	20	3.8	4.8	4.9	5	0.1	2.0	6.2	20	>6
<a href="#">Lab040</a>	5	14.4	12.8	1	-	-	-	20	-	5.8	4.5	1	-	-	-	20	-
Total	-	-	13.5	24	1.2	8.9	-	-	-	-	4.9	24	0.2	4.1	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

## Cumulative

Cumulative : from 2016  02  01  to 2020  07  31

		Control N (Lot No.: AE0909N)								Control D (Lot No.: AE0909D)							
UnitID <input type="button" value="↑"/>	Reagent Kit (Code) <input type="button" value="↑"/>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	14.2	14.9	142	1.2	8.1	21.0	20	1.9	5.5	5.5	142	0.3	5.5	10.9	20	3.6
<a href="#">Lab019</a>	5	15.3	15.2	111	0.3	2.0	4.6	20	>6	5.3	5.3	111	0.2	3.8	7.5	20	5.3
<a href="#">Lab020</a>	5	14.4	15.2	28	0.5	3.3	12.1	20	4.4	5.8	5.3	28	0.3	5.7	19.9	20	2.0
<a href="#">Lab026</a>	5	15.9	13.6	368	1.3	9.6	33.6	20	0.6	5.8	5.1	368	0.3	5.9	23.8	20	1.3
<a href="#">Lab027</a>	5	15.5	15.5	107	1.3	8.4	16.8	20	2.4	5.4	5.6	107	0.5	8.9	21.6	20	1.8
<a href="#">Lab028</a>	5	14.8	14.5	134	0.7	4.8	11.7	20	3.7	4.8	5.6	134	0.3	5.4	27.4	20	0.6
<a href="#">Lab032</a>	5	15.3	15.9	38	0.9	5.7	15.2	20	2.8	5.2	5.7	38	0.3	5.3	20.1	20	2.0
<a href="#">Lab033</a>	5	14.4	14.9	49	0.6	4.0	11.5	20	4.1	5.8	5.2	49	0.2	3.8	18.0	20	2.5
<a href="#">Lab034</a>	5	15.5	14.7	96	0.9	6.1	17.4	20	2.4	4.8	5.0	96	0.4	8.0	20.2	20	2.0
<a href="#">Lab037</a>	5	14.9	15.2	30	0.8	5.3	12.5	20	3.4	5.4	5.5	30	0.3	5.5	12.8	20	3.3
<a href="#">Lab040</a>	5	14.4	13.2	40	0.7	5.3	18.9	20	2.2	5.8	4.7	40	0.3	6.4	31.7	20	0.2
<a href="#">Lab043</a>	5	11.5	13.1	84	0.9	6.9	27.7	20	0.9	4.5	4.9	84	0.3	6.1	21.1	20	1.8
Total	-	-	14.4	1227	1.3	9.0	-	-	-	-	5.3	1227	0.4	7.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

Reagent Kit	Reagent Code
Medicon	5

## Peer Group Statistics (Table 2)

Select LotNo : AE0909N (2016-01-01 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

Print Table 2

### Control N Month vs. Cumulative

Control N (Lot No.: AE0909N)																	
		Month (2020/07)								CUM (2016/02/01~2020/07/31)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	14.2	-	0	-	-	-	20	-	14.2	14.9	142	1.2	8.1	21.0	20	1.9
<a href="#">Lab019</a>	5	15.3	14.9	1	-	-	-	20	-	15.3	15.2	111	0.3	2.0	4.6	20	>6
<a href="#">Lab020</a>	5	14.4	-	0	-	-	-	20	-	14.4	15.2	28	0.5	3.3	12.1	20	4.4
<a href="#">Lab026</a>	5	15.9	12.9	17	0.1	0.8	20.4	20	1.4	15.9	13.6	368	1.3	9.6	33.6	20	0.6
<a href="#">Lab027</a>	5	15.5	-	0	-	-	-	20	-	15.5	15.5	107	1.3	8.4	16.8	20	2.4
<a href="#">Lab028</a>	5	14.8	-	0	-	-	-	20	-	14.8	14.5	134	0.7	4.8	11.7	20	3.7
<a href="#">Lab032</a>	5	15.3	-	0	-	-	-	20	-	15.3	15.9	38	0.9	5.7	15.2	20	2.8
<a href="#">Lab033</a>	5	14.4	-	0	-	-	-	20	-	14.4	14.9	49	0.6	4.0	11.5	20	4.1
<a href="#">Lab034</a>	5	15.5	15.5	5	0.8	5.2	10.3	20	3.8	15.5	14.7	96	0.9	6.1	17.4	20	2.4
<a href="#">Lab037</a>	5	14.9	-	0	-	-	-	20	-	14.9	15.2	30	0.8	5.3	12.5	20	3.4
<a href="#">Lab040</a>	5	14.4	12.8	1	-	-	-	20	-	14.4	13.2	40	0.7	5.3	18.9	20	2.2
<a href="#">Lab043</a>	5	11.5	-	0	-	-	-	20	-	11.5	13.1	84	0.9	6.9	27.7	20	0.9
Total	-	-	13.5	24	1.2	8.9	-	-	-	-	14.4	1227	1.3	9.0	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2020 07 Change

Cumulative : from 2016 02 01 to 2020 07 31 Change

[TOP](#)

### Control D Month vs. Cumulative

Control D (Lot No.: AE0909D)																	
		Month (2020/07)								CUM (2016/02/01~2020/07/31)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	5.5	-	0	-	-	-	20	-	5.5	5.5	142	0.3	5.5	10.9	20	3.6
<a href="#">Lab019</a>	5	5.3	4.8	1	-	-	-	20	-	5.3	5.3	111	0.2	3.8	7.5	20	5.3
<a href="#">Lab020</a>	5	5.8	-	0	-	-	-	20	-	5.8	5.3	28	0.3	5.7	19.9	20	2.0
<a href="#">Lab026</a>	5	5.8	4.9	17	0.2	4.1	23.7	20	1.1	5.8	5.1	368	0.3	5.9	23.8	20	1.3
<a href="#">Lab027</a>	5	5.4	-	0	-	-	-	20	-	5.4	5.6	107	0.5	8.9	21.6	20	1.8
<a href="#">Lab028</a>	5	4.8	-	0	-	-	-	20	-	4.8	5.6	134	0.3	5.4	27.4	20	0.6
<a href="#">Lab032</a>	5	5.2	-	0	-	-	-	20	-	5.2	5.7	38	0.3	5.3	20.1	20	2.0
<a href="#">Lab033</a>	5	5.8	-	0	-	-	-	20	-	5.8	5.2	49	0.2	3.8	18.0	20	2.5
<a href="#">Lab034</a>	5	4.8	4.9	5	0.1	2.0	6.2	20	>6	4.8	5.0	96	0.4	8.0	20.2	20	2.0
<a href="#">Lab037</a>	5	5.4	-	0	-	-	-	20	-	5.4	5.5	30	0.3	5.5	12.8	20	3.3
<a href="#">Lab040</a>	5	5.8	4.5	1	-	-	-	20	-	5.8	4.7	40	0.3	6.4	31.7	20	0.2
<a href="#">Lab043</a>	5	4.5	-	0	-	-	-	20	-	4.5	4.9	84	0.3	6.1	21.1	20	1.8
Total	-	-	4.9	24	0.2	4.1	-	-	-	-	5.3	1227	0.4	7.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2020 07 Change

Cumulative : from 2016 02 01 to 2020 07 31 Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5