

# QC Chart of Internal Quality Control (IQC) for G6PD Quantitative Test

Select LotNo : BA1116N (2022-04-26 ~ 2100-12-31) Change

[Print Table](#)

## Lab037

QC Control Lot No.	Control N		Control D	
	BA1116N		BA1116D	
Duration of the Analyzing	Month (2024/02)	CUM (2023/07/28~2024/02/29)	Month (2024/02)	CUM (2023/07/28~2024/02/29)
Runs (N)	2	12	2	12
Mean (U/gHb)	14.1	14.0	4.5	4.5
SD	-	0.4	-	0.1
CV (%)	-	2.9	-	2.2
Target Value (U/gHb)	12.8	12.8	4.2	4.2
Total Error (%)	-	15.1	-	11.6
TEa (%)	20	20	20	20
$\sigma$	-	3.7	-	5.8

Bias (%) =  $[ ( | \text{Mean} - \text{Target} | ) / \text{Target} ] \times 100\%$   
 TE : Total Error(%) = Bias (%) + 2 × CV (%)  
 $\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2024 02 Change ; Cumulative : from 2023 07 28 to 2024 02 29 Change


[TOP](#)

## Control N and Control D SDI QC Chart

Lot No.: BA1116N ; Duration : 2023-07-28 to 2024-02-29 ; Target : 12.8 ; SD : 1.28 (●)

Lot No.: BA1116D ; Duration : 2023-07-28 to 2024-02-29 ; Target : 4.2 ; SD : 0.42 (□)

Lab037

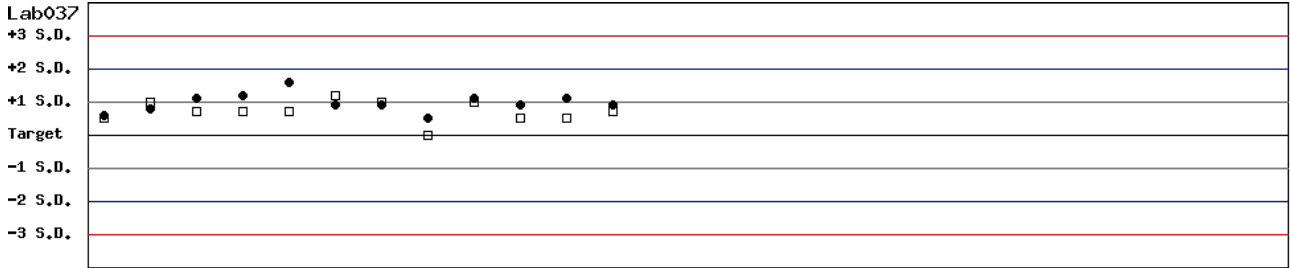

Date 07-28 08-24 09-08 09-29 10-12 10-26 11-09 11-24 01-10 01-25 02-08 02-23


Month : 2024 02 Change ; Cumulative : from 2023 07 28 to 2024 02 29 Change

[TOP](#)

## Control N SDI QC Chart

Lot No.: BA1116N ; Duration : 2023-07-28 to 2024-02-29 ; Target : 12.8 ; SD : 1.28

Lab037

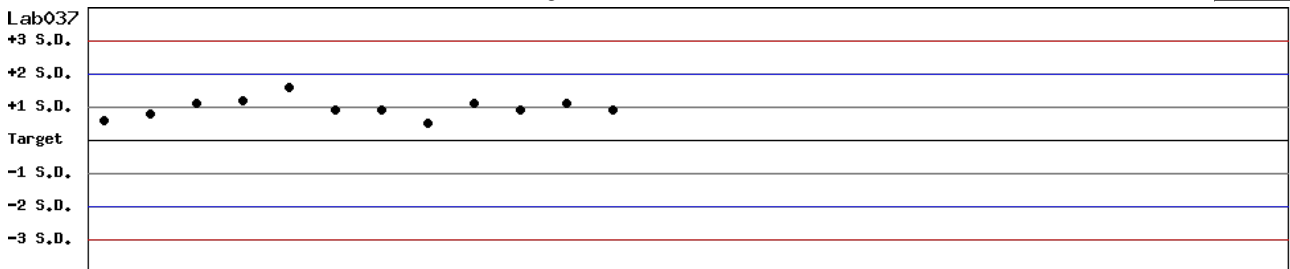

Date 07-28 08-24 09-08 09-29 10-12 10-26 11-09 11-24 01-10 01-25 02-08 02-23

Month : 2024 02 Change ; Cumulative : from 2023 07 28 to 2024 02 29 Change

[TOP](#)

### Control D SDI QC Chart

Lot No.: BA1116D ; Duration : 2023-07-28 to 2024-02-29 ; Target : 4.2 ; SD : 0.42

Lab037



Date 07-28 08-24 09-08 09-29 10-12 10-26 11-09 11-24 01-10 01-25 02-08 02-23

Month : 2024 v 02 v Change ; Cumulative : from 2023 v 07 v 28 v to 2024 v 02 v 29 v Change

[TOP](#)

# Peer Group Statistics (Table 1)

Select LotNo : BA1116N (2022-04-26 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

[Print Table 1](#)

## Monthly

Month : 2024 02 Change

UnitID <span>↑</span>	Reagent Kit (Code) <span>↑</span>	Control N (Lot No.: BA1116N)								Control D (Lot No.: BA1116D)							
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab027</a>	5	12.8	14.9	2	-	-	-	20	-	4.2	5.7	2	-	-	-	20	-
<a href="#">Lab033</a>	5	15.8	16.0	5	0.3	1.9	5.0	20	>6	4.2	4.9	5	0.2	4.1	24.8	20	0.8
<a href="#">Lab037</a>	5	12.8	14.1	2	-	-	-	20	-	4.2	4.5	2	-	-	-	20	-
Total	-	-	15.3	9	1.0	6.5	-	-	-	-	5.0	9	0.5	10.0	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

## Cumulative

Cumulative : from 2022 06 01 to 2024 02 29 Change

UnitID <span>↑</span>	Reagent Kit (Code) <span>↑</span>	Control N (Lot No.: BA1116N)								Control D (Lot No.: BA1116D)							
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	13.6	13.8	113	0.4	2.9	7.3	20	>6	4.3	4.4	113	0.1	2.3	6.9	20	>6
<a href="#">Lab027</a>	5	12.8	14.9	74	0.9	6.0	28.5	20	0.6	4.2	4.9	74	0.4	8.2	33.0	20	0.4
<a href="#">Lab033</a>	5	15.8	15.9	31	0.6	3.8	8.2	20	5.1	4.2	4.8	31	0.3	6.3	26.8	20	0.9
<a href="#">Lab037</a>	5	12.8	14.0	12	0.4	2.9	15.1	20	3.7	4.2	4.5	12	0.1	2.2	11.6	20	5.8
Total	-	-	14.4	230	1.0	6.9	-	-	-	-	4.6	230	0.3	6.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

Reagent Kit	Reagent Code
Medicon	5

## Peer Group Statistics (Table 2)

Select LotNo : BA1116N (2022-04-26 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

Print Table 2

### Control N Month vs. Cumulative

		Control N (Lot No.: BA1116N)															
		Month (2024/02)								CUM (2022/06/01~2024/02/29)							
UnitID <span>↑</span>	Reagent Kit (Code) <span>↑</span>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	13.6	-	0	-	-	-	20	-	13.6	13.8	113	0.4	2.9	7.3	20	>6
<a href="#">Lab027</a>	5	12.8	14.9	2	-	-	-	20	-	12.8	14.9	74	0.9	6.0	28.5	20	0.6
<a href="#">Lab033</a>	5	15.8	16.0	5	0.3	1.9	5.0	20	>6	15.8	15.9	31	0.6	3.8	8.2	20	5.1
<a href="#">Lab037</a>	5	12.8	14.1	2	-	-	-	20	-	12.8	14.0	12	0.4	2.9	15.1	20	3.7
<b>Total</b>	-	-	15.3	9	1.0	6.5	-	-	-	-	14.4	230	1.0	6.9	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2024 02 Change    Cumulative : from 2022 06 01 to 2024 02 29 Change

[TOP](#)

### Control D Month vs. Cumulative

		Control D (Lot No.: BA1116D)															
		Month (2024/02)								CUM (2022/06/01~2024/02/29)							
UnitID <span>↑</span>	Reagent Kit (Code) <span>↑</span>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	4.3	-	0	-	-	-	20	-	4.3	4.4	113	0.1	2.3	6.9	20	>6
<a href="#">Lab027</a>	5	4.2	5.7	2	-	-	-	20	-	4.2	4.9	74	0.4	8.2	33.0	20	0.4
<a href="#">Lab033</a>	5	4.2	4.9	5	0.2	4.1	24.8	20	0.8	4.2	4.8	31	0.3	6.3	26.8	20	0.9
<a href="#">Lab037</a>	5	4.2	4.5	2	-	-	-	20	-	4.2	4.5	12	0.1	2.2	11.6	20	5.8
<b>Total</b>	-	-	5.0	9	0.5	10.0	-	-	-	-	4.6	230	0.3	6.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2024 02 Change    Cumulative : from 2022 06 01 to 2024 02 29 Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5