

# Summary Report of IQC program for G6PD Quantitative Test - Medicon Group - June 2024 -



## I. The statistic results of all laboratories in this month

G6PD	Control N (Lot No.:BJ0922N)	Control D (Lot No.: BJ0922D)
Labs	8	8
Received results number (n)	40	40
Median	14.8 (U/g Hb)	5.1 (U/g Hb)
Mean	14.7 (U/g Hb)	5.1 (U/g Hb)
SD	0.5	0.3
CV	3.4%	5.9%
Range of G6PD	13.5 ~ 15.4 (U/g Hb)	4.4 ~ 5.8 (U/g Hb)
Range of Hb	1.9 ~ 2.6 (g/dL)	1.7 ~ 2.2 (g/dL)

\*The statistic results are calculated from all labs reported in this month

\*\* G6PD Method = Medicon reagent kit, 37°C

## II. The distribution of G6PD reported for each lab in this survey

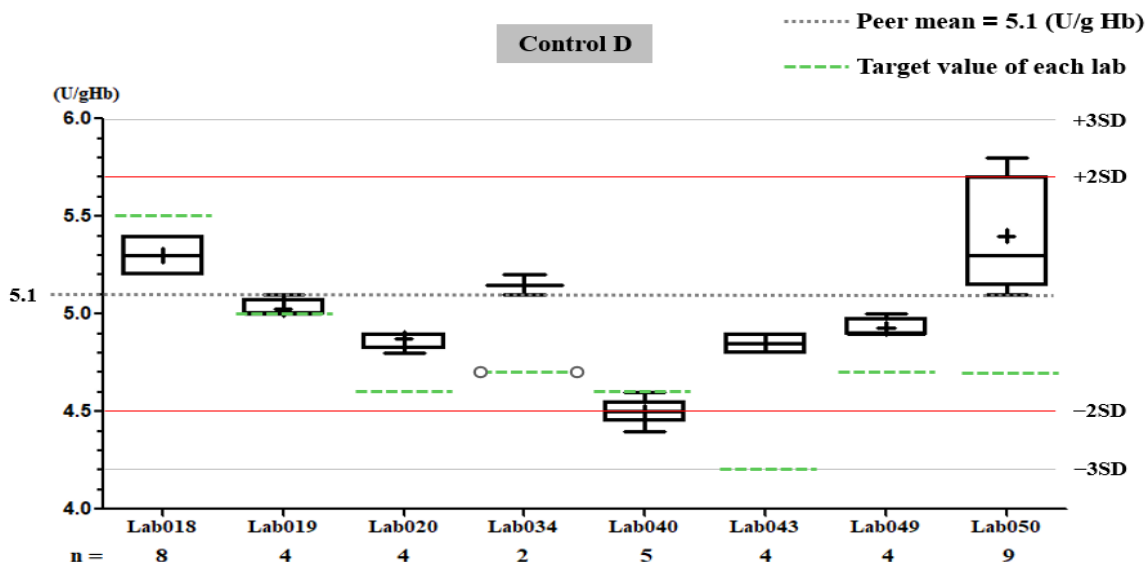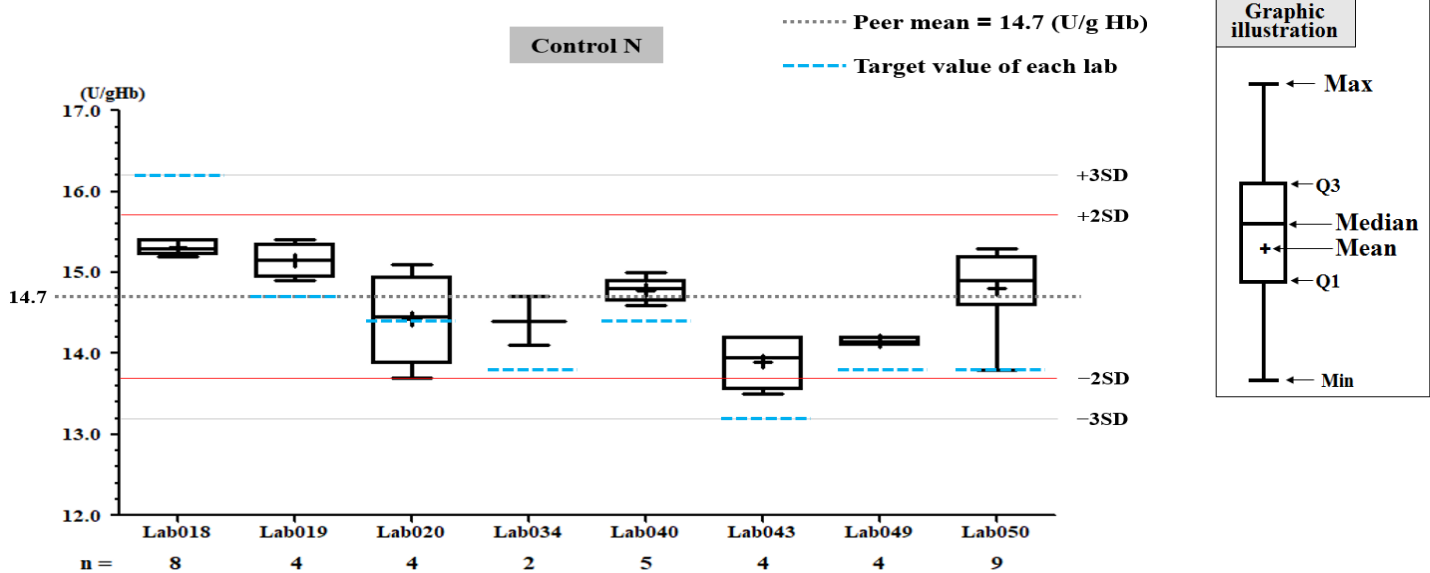

# QC Chart of Internal Quality Control (IQC) for G6PD Quantitative Test

Select LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) Change

[Print Table](#)

## Lab019

QC Control Lot No.	Control N		Control D	
	BJ0922N		BJ0922D	
Duration of the Analyzing	Month (2024/06)	CUM (2024/01/03~2024/06/30)	Month (2024/06)	CUM (2024/01/03~2024/06/30)
Runs (N)	4	26	4	26
Mean (U/gHb)	15.2	14.8	5.0	5.0
SD	0.2	0.3	0.1	0.1
CV (%)	1.3	2.0	2.0	2.0
Target Value (U/gHb)	14.7	14.7	5.0	5.0
Total Error (%)	6.0	4.7	4.0	4.0
TEa (%)	20	20	20	20
$\sigma$	>6	>6	>6	>6

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 $\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2024 06 Change ; Cumulative : from 2024 01 03 to 2024 06 30 Change


[\[TOP\]](#)

## Control N and Control D SDI QC Chart

Lot No.: BJ0922N ; Duration : 2024-01-03 to 2024-06-30 ; Target : 14.7 ; SD : 0.90 (●)

Lot No.: BJ0922D ; Duration : 2024-01-03 to 2024-06-30 ; Target : 5.0 ; SD : 0.30 (□)

Lab019

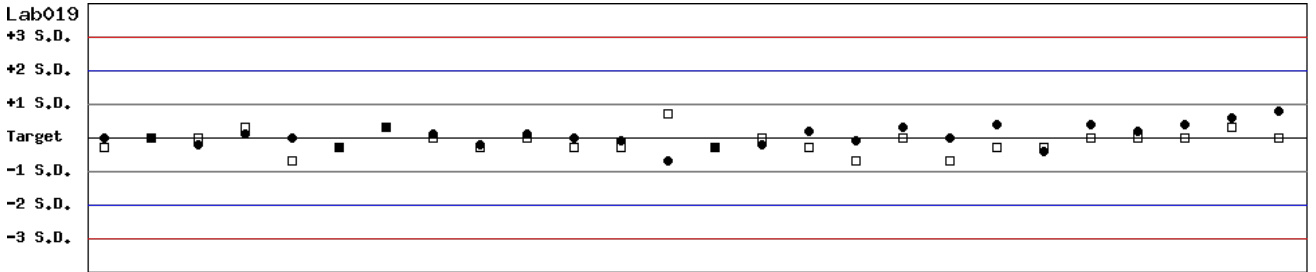

Date 01-03 01-10 01-17 01-24 01-31 02-07 02-14 02-21 02-28 03-06 03-13 03-20 03-27 04-03 04-10 04-17 04-24 05-01 05-08 05-15 05-22 05-29 06-05 06-12 06-19 06-26


Month : 2024 06 Change ; Cumulative : from 2024 01 03 to 2024 06 30 Change

[\[TOP\]](#)

## Control N SDI QC Chart

Lot No.: BJ0922N ; Duration : 2024-01-03 to 2024-06-30 ; Target : 14.7 ; SD : 0.90

Lab019

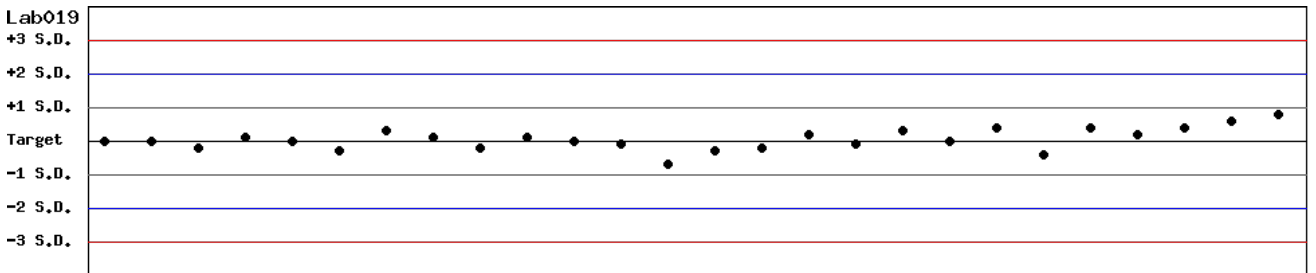

Date 01-03 01-10 01-17 01-24 01-31 02-07 02-14 02-21 02-28 03-06 03-13 03-20 03-27 04-03 04-10 04-17 04-24 05-01 05-08 05-15 05-22 05-29 06-05 06-12 06-19 06-26


Month : 2024 06 Change ; Cumulative : from 2024 01 03 to 2024 06 30 Change

[\[TOP\]](#)

# Control D SDI QC Chart

Lab019

Lot No.: BJ0922D ; Duration : 2024-01-03 to 2024-06-30 ; Target : 5.0 ; SD : 0.30

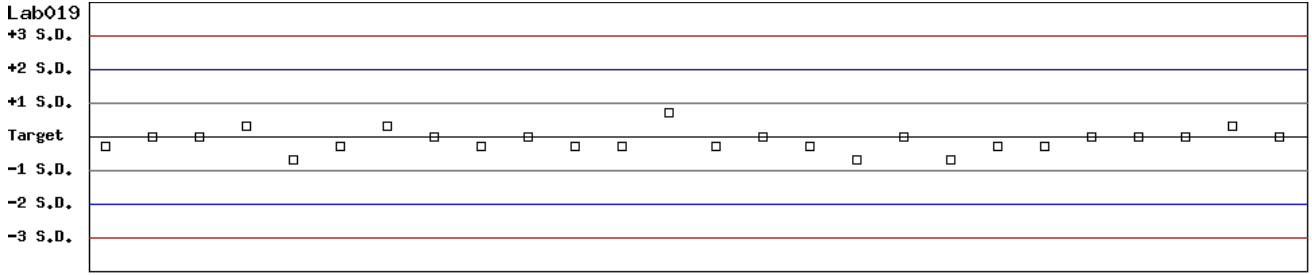

Date 01-03 01-10 01-17 01-24 01-31 02-07 02-14 02-21 02-28 03-06 03-13 03-20 03-27 04-03 04-10 04-17 04-24 05-01 05-08 05-15 05-22 05-29 06-05 06-12 06-19 06-26

Month : 2024 v 06 v Change ; Cumulative : from 2024 v 01 v 03 v to 2024 v 06 v 30 v Change

[TOP](#)

# Peer Group Statistics (Table 1)

Select LotNo : BJ0922N (2021-01-01 ~ 2100-12-31)

Select Reagent Kit : 5 - Medicon

## Monthly

Month : 2024  06

UnitID <input type="button" value="↑"/>	Reagent Kit (Code) <input type="button" value="↑"/>	Control N (Lot No.: BJ0922N)								Control D (Lot No.: BJ0922D)							
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	16.2	15.3	8	0.1	0.7	6.9	20	>6	5.5	5.3	8	0.1	1.9	7.4	20	>6
<a href="#">Lab019</a>	5	14.7	15.2	4	0.2	1.3	6.0	20	>6	5.0	5.0	4	0.1	2.0	4.0	20	>6
<a href="#">Lab020</a>	5	14.4	14.4	4	0.6	4.2	8.3	20	4.8	4.6	4.9	4	0.1	2.0	10.6	20	>6
<a href="#">Lab034</a>	5	13.8	14.4	2	-	-	-	20	-	4.7	5.2	2	-	-	-	20	-
<a href="#">Lab040</a>	5	14.4	14.8	5	0.2	1.4	5.5	20	>6	4.6	4.5	5	0.1	2.2	6.6	20	>6
<a href="#">Lab043</a>	5	13.2	13.9	4	0.4	2.9	11.1	20	5.1	4.2	4.9	4	0.1	2.0	20.7	20	1.7
<a href="#">Lab049</a>	5	13.8	14.2	4	0.1	0.7	4.3	20	>6	4.7	4.9	4	0.1	2.0	8.3	20	>6
<a href="#">Lab050</a>	5	13.8	14.8	9	0.5	3.4	14.0	20	3.8	4.7	5.4	9	0.3	5.6	26.0	20	0.9
Total	-	-	14.7	40	0.5	3.4	-	-	-	-	5.1	40	0.3	5.9	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

## Cumulative

Cumulative : from 2021  01  01 to 2024  06  30

UnitID <input type="button" value="↑"/>	Reagent Kit (Code) <input type="button" value="↑"/>	Control N (Lot No.: BJ0922N)								Control D (Lot No.: BJ0922D)							
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	16.2	15.3	86	0.4	2.6	10.8	20	5.6	5.5	5.4	86	0.1	1.9	5.5	20	>6
<a href="#">Lab019</a>	5	14.7	14.5	118	0.6	4.1	9.6	20	4.5	5.0	4.8	118	0.3	6.3	16.5	20	2.5
<a href="#">Lab020</a>	5	14.4	14.4	89	0.5	3.5	6.9	20	5.7	4.6	4.7	89	0.2	4.3	10.7	20	4.1
<a href="#">Lab022</a>	5	14.4	14.4	27	0.5	3.5	6.9	20	5.7	4.6	4.7	27	0.3	6.4	14.9	20	2.8
<a href="#">Lab028</a>	5	15.2	15.1	34	1.1	7.3	15.2	20	2.6	4.9	4.9	34	0.3	6.1	12.2	20	3.3
<a href="#">Lab032</a>	5	14.9	14.3	153	0.4	2.8	9.6	20	5.7	4.8	4.5	153	0.2	4.4	15.1	20	3.1
<a href="#">Lab033</a>	5	13.8	13.6	81	0.7	5.1	11.7	20	3.6	4.7	4.6	81	0.3	6.5	15.2	20	2.7
<a href="#">Lab034</a>	5	13.8	14.4	11	0.4	2.8	9.9	20	5.6	4.7	5.2	11	0.2	3.8	18.3	20	2.5
<a href="#">Lab037</a>	5	13.8	14.5	59	0.5	3.4	12.0	20	4.4	4.7	4.7	59	0.2	4.3	8.5	20	4.7
<a href="#">Lab040</a>	5	14.4	14.8	114	0.2	1.4	5.5	20	>6	4.6	4.6	114	0.1	2.2	4.3	20	>6
<a href="#">Lab043</a>	5	13.2	13.9	145	1.1	7.9	21.1	20	1.9	4.2	4.6	145	0.4	8.7	26.9	20	1.2
<a href="#">Lab049</a>	5	13.8	14.4	215	0.6	4.2	12.7	20	3.7	4.7	4.7	215	0.3	6.4	12.8	20	3.1
<a href="#">Lab050</a>	5	13.8	14.5	29	0.6	4.1	13.3	20	3.6	4.7	5.3	29	0.3	5.7	24.1	20	1.3
Total	-	-	14.4	1161	0.7	4.9	-	-	-	-	4.7	1161	0.3	6.4	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5

## Peer Group Statistics (Table 2)

Select LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

Print Table 2

### Control N Month vs. Cumulative

		Control N (Lot No.: BJ0922N)															
		Month (2024/06)									CUM (2021/01/01~2024/06/30)						
UnitID <span style="font-size: small;">↑</span>	Reagent Kit (Code) <span style="font-size: small;">↑</span>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	16.2	15.3	8	0.1	0.7	6.9	20	>6	16.2	15.3	86	0.4	2.6	10.8	20	5.6
<a href="#">Lab019</a>	5	14.7	15.2	4	0.2	1.3	6.0	20	>6	14.7	14.5	118	0.6	4.1	9.6	20	4.5
<a href="#">Lab020</a>	5	14.4	14.4	4	0.6	4.2	8.3	20	4.8	14.4	14.4	89	0.5	3.5	6.9	20	5.7
<a href="#">Lab022</a>	5	14.4	-	0	-	-	-	20	-	14.4	14.4	27	0.5	3.5	6.9	20	5.7
<a href="#">Lab028</a>	5	15.2	-	0	-	-	-	20	-	15.2	15.1	34	1.1	7.3	15.2	20	2.6
<a href="#">Lab032</a>	5	14.9	-	0	-	-	-	20	-	14.9	14.3	153	0.4	2.8	9.6	20	5.7
<a href="#">Lab033</a>	5	13.8	-	0	-	-	-	20	-	13.8	13.6	81	0.7	5.1	11.7	20	3.6
<a href="#">Lab034</a>	5	13.8	14.4	2	-	-	-	20	-	13.8	14.4	11	0.4	2.8	9.9	20	5.6
<a href="#">Lab037</a>	5	13.8	-	0	-	-	-	20	-	13.8	14.5	59	0.5	3.4	12.0	20	4.4
<a href="#">Lab040</a>	5	14.4	14.8	5	0.2	1.4	5.5	20	>6	14.4	14.8	114	0.2	1.4	5.5	20	>6
<a href="#">Lab043</a>	5	13.2	13.9	4	0.4	2.9	11.1	20	5.1	13.2	13.9	145	1.1	7.9	21.1	20	1.9
<a href="#">Lab049</a>	5	13.8	14.2	4	0.1	0.7	4.3	20	>6	13.8	14.4	215	0.6	4.2	12.7	20	3.7
<a href="#">Lab050</a>	5	13.8	14.8	9	0.5	3.4	14.0	20	3.8	13.8	14.5	29	0.6	4.1	13.3	20	3.6
Total	-	-	14.7	40	0.5	3.4	-	-	-	-	14.4	1161	0.7	4.9	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2024 06 Change

Cumulative : from 2021 01 01 to 2024 06 30 Change

[TOP](#)

### Control D Month vs. Cumulative

		Control D (Lot No.: BJ0922D)															
		Month (2024/06)									CUM (2021/01/01~2024/06/30)						
UnitID <span style="font-size: small;">↑</span>	Reagent Kit (Code) <span style="font-size: small;">↑</span>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	5.5	5.3	8	0.1	1.9	7.4	20	>6	5.5	5.4	86	0.1	1.9	5.5	20	>6
<a href="#">Lab019</a>	5	5.0	5.0	4	0.1	2.0	4.0	20	>6	5.0	4.8	118	0.3	6.3	16.5	20	2.5
<a href="#">Lab020</a>	5	4.6	4.9	4	0.1	2.0	10.6	20	>6	4.6	4.7	89	0.2	4.3	10.7	20	4.1
<a href="#">Lab022</a>	5	4.6	-	0	-	-	-	20	-	4.6	4.7	27	0.3	6.4	14.9	20	2.8
<a href="#">Lab028</a>	5	4.9	-	0	-	-	-	20	-	4.9	4.9	34	0.3	6.1	12.2	20	3.3
<a href="#">Lab032</a>	5	4.8	-	0	-	-	-	20	-	4.8	4.5	153	0.2	4.4	15.1	20	3.1
<a href="#">Lab033</a>	5	4.7	-	0	-	-	-	20	-	4.7	4.6	81	0.3	6.5	15.2	20	2.7
<a href="#">Lab034</a>	5	4.7	5.2	2	-	-	-	20	-	4.7	5.2	11	0.2	3.8	18.3	20	2.5
<a href="#">Lab037</a>	5	4.7	-	0	-	-	-	20	-	4.7	4.7	59	0.2	4.3	8.5	20	4.7
<a href="#">Lab040</a>	5	4.6	4.5	5	0.1	2.2	6.6	20	>6	4.6	4.6	114	0.1	2.2	4.3	20	>6
<a href="#">Lab043</a>	5	4.2	4.9	4	0.1	2.0	20.7	20	1.7	4.2	4.6	145	0.4	8.7	26.9	20	1.2
<a href="#">Lab049</a>	5	4.7	4.9	4	0.1	2.0	8.3	20	>6	4.7	4.7	215	0.3	6.4	12.8	20	3.1
<a href="#">Lab050</a>	5	4.7	5.4	9	0.3	5.6	26.0	20	0.9	4.7	5.3	29	0.3	5.7	24.1	20	1.3
Total	-	-	5.1	40	0.3	5.9	-	-	-	-	4.7	1161	0.3	6.4	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2024 06 Change

Cumulative : from 2021 01 01 to 2024 06 30 Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5