

QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : BA1116N (2022-04-26 ~ 2100-12-31) Change

Print Table

Lab052

	Control N		Control D	
QC Control Lot No.	BA1116N		BA1116D	
Duration of the Analyzing	Month (2025/02)	CUM (2022/06/01~2025/02/28)	Month (2025/02)	CUM (2022/06/01~2025/02/28)
Runs (N)	5	18	5	18
Mean (U/gHb)	15.3	15.3	4.7	4.7
SD	0.5	0.4	0.2	0.2
CV (%)	3.3	2.6	4.3	4.3
Target Value (U/gHb)	15.3	15.3	4.6	4.6
Total Error (%)	6.5	5.2	10.7	10.7
TEa (%)	20	20	20	20
σ	>6	>6	4.1	4.1

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2025 02 Change ; Cumulative : from 2022 06 01 to 2025 02 28 Change

TOP


Control N and Control D SDI QC Chart

Lot No.: BA1116N ; Duration : 2022-06-01 to 2025-02-28 ; Target : 15.3 ; SD : 0.35 (●)

Lot No.: BA1116D ; Duration : 2022-06-01 to 2025-02-28 ; Target : 4.6 ; SD : 0.21 (□)

Lab052

Lab052
+3 S.D.
+2 S.D.
+1 S.D.
Target
-1 S.D.
-2 S.D.
-3 S.D.

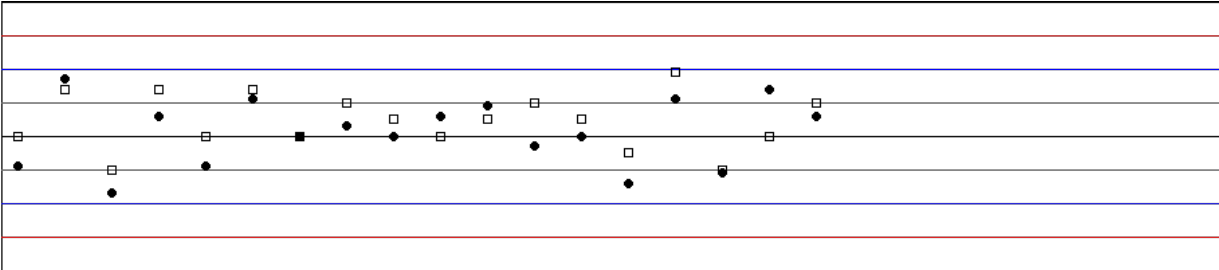

Date 10-03 10-10 10-18 10-24 10-31 11-07 11-14 11-21 11-28 12-06 12-12 12-19 01-30 02-06 02-13 02-20 02-22 02-27

Month : 2025 02 Change ; Cumulative : from 2022 06 01 to 2025 02 28 Change


TOP

Control N SDI QC Chart

Lot No.: BA1116N ; Duration : 2022-06-01 to 2025-02-28 ; Target : 15.3 ; SD : 0.35

Lab052

Lab052
+3 S.D.
+2 S.D.
+1 S.D.
Target
-1 S.D.
-2 S.D.
-3 S.D.

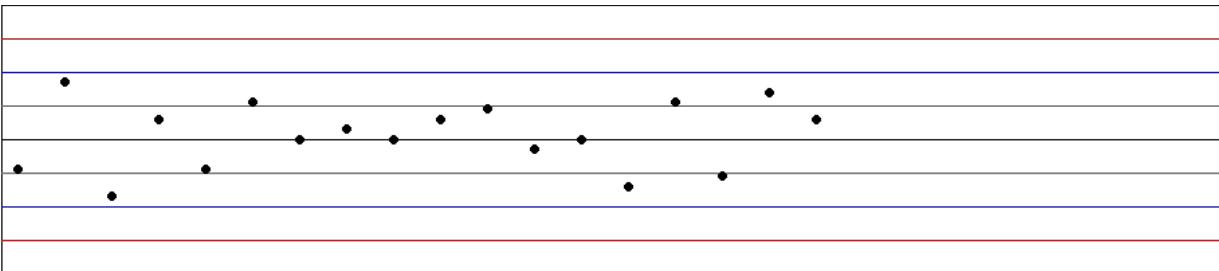

Date 10-03 10-10 10-18 10-24 10-31 11-07 11-14 11-21 11-28 12-06 12-12 12-19 01-30 02-06 02-13 02-20 02-22 02-27

Month : 2025 02 Change ; Cumulative : from 2022 06 01 to 2025 02 28 Change


TOP

Control D SDI QC Chart

Lab052

Lot No.: BA1116D ; Duration : 2022-06-01 to 2025-02-28 ; Target : 4.6 ; SD : 0.21

Lab052
+3 S.D.
+2 S.D.
+1 S.D.
Target
-1 S.D.
-2 S.D.
-3 S.D.

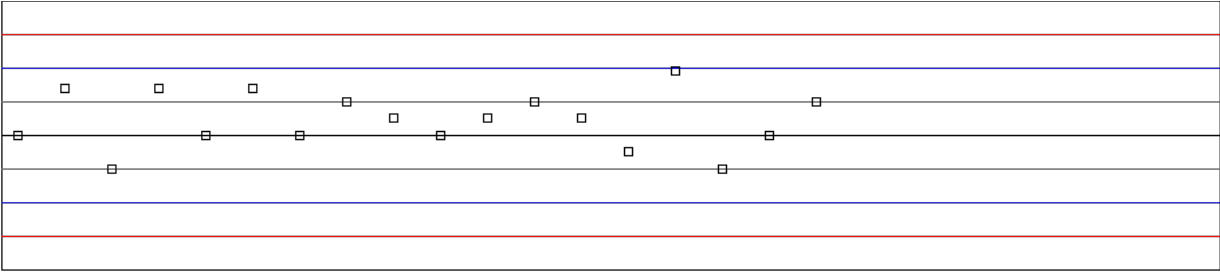

Date 10-03 10-10 10-18 10-24 10-31 11-07 11-14 11-21 11-28 12-06 12-12 12-19 01-30 02-06 02-13 02-20 02-22 02-27

Month : 2025 02 Change ; Cumulative : from 2022 06 01 to 2025 02 28 Change

[\[TOP\]](#)

Peer Group Statistics (Table 1)

Select LotNo : BA1116N (2022-04-26 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

[Print Table 1](#)

Monthly

Month : 2025 02 Change

		Control N (Lot No.: BA1116N)									Control D (Lot No.: BA1116D)							
UnitID 	Reagent Kit (Code) 	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab032	5	14.9	14.3	4	0.1	0.7	5.4	20	>6		5.1	4.4	4	0.1	2.3	18.3	20	2.7
Lab033	5	15.8	15.0	4	0.4	2.7	10.4	20	5.5		4.7	4.6	4	0.1	2.2	6.5	20	>6
Lab037	5	12.8	13.9	2	-	-	-	20	-		4.2	4.6	2	-	-	-	20	-
Lab052	5	15.3	15.3	5	0.5	3.3	6.5	20	>6		4.6	4.7	5	0.2	4.3	10.7	20	4.1
Total	-	-	14.7	15	0.6	4.1	-	-	-		-	4.6	15	0.2	4.3	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[\[TOP\]](#)

Cumulative

Cumulative : from 2022 06 01 to 2025 02 28 Change

		Control N (Lot No.: BA1116N)									Control D (Lot No.: BA1116D)							
UnitID 	Reagent Kit (Code) 	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab018	5	13.6	13.8	139	0.4	2.9	7.3	20	>6		4.3	4.4	139	0.1	2.3	6.9	20	>6
Lab027	5	12.8	14.9	74	0.9	6.0	28.5	20	0.6		4.2	4.9	74	0.4	8.2	33.0	20	0.4
Lab032	5	14.9	13.8	26	0.4	2.9	13.2	20	4.4		5.1	4.3	26	0.2	4.7	25.0	20	0.9
Lab033	5	15.8	15.7	83	0.6	3.8	8.3	20	5.1		4.7	4.8	83	0.2	4.2	10.5	20	4.3
Lab037	5	12.8	13.8	35	0.4	2.9	13.6	20	4.2		4.2	4.4	35	0.2	4.5	13.9	20	3.4
Lab052	5	15.3	15.4	14	0.3	1.9	4.5	20	>6		4.6	4.7	14	0.2	4.3	10.7	20	4.1
Total	-	-	14.5	375	1.0	6.9	-	-	-		-	4.6	375	0.3	6.5	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[\[TOP\]](#)

Reagent Kit	Reagent Code
Medicon	5

Peer Group Statistics (Table 2)

Select LotNo : BA1116N (2022-04-26 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

Print Table 2

Control N Month vs. Cumulative

Control N (Lot No.: BA1116N)																	
Month (2025/02)										CUM (2022/06/01~2025/02/28)							
UnitID 	Reagent Kit (Code) 	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab018	5	13.6	-	0	-	-	-	20	-	13.6	13.8	139	0.4	2.9	7.3	20	>6
Lab027	5	12.8	-	0	-	-	-	20	-	12.8	14.9	74	0.9	6.0	28.5	20	0.6
Lab032	5	14.9	14.3	4	0.1	0.7	5.4	20	>6	14.9	13.8	26	0.4	2.9	13.2	20	4.4
Lab033	5	15.8	15.0	4	0.4	2.7	10.4	20	5.5	15.8	15.7	83	0.6	3.8	8.3	20	5.1
Lab037	5	12.8	13.9	2	-	-	-	20	-	12.8	13.8	35	0.4	2.9	13.6	20	4.2
Lab052	5	15.3	15.3	5	0.5	3.3	6.5	20	>6	15.3	15.4	14	0.3	1.9	4.5	20	>6
Total	-	-	14.7	15	0.6	4.1	-	-	-	-	14.5	375	1.0	6.9	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE : Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2025 02 Change Cumulative : from 2022 06 01 to 2025 02 28 Change

[TOP](#)

Control D Month vs. Cumulative

Control D (Lot No.: BA1116D)																	
Month (2025/02)										CUM (2022/06/01~2025/02/28)							
UnitID 	Reagent Kit (Code) 	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab018	5	4.3	-	0	-	-	-	20	-	4.3	4.4	139	0.1	2.3	6.9	20	>6
Lab027	5	4.2	-	0	-	-	-	20	-	4.2	4.9	74	0.4	8.2	33.0	20	0.4
Lab032	5	5.1	4.4	4	0.1	2.3	18.3	20	2.7	5.1	4.3	26	0.2	4.7	25.0	20	0.9
Lab033	5	4.7	4.6	4	0.1	2.2	6.5	20	>6	4.7	4.8	83	0.2	4.2	10.5	20	4.3
Lab037	5	4.2	4.6	2	-	-	-	20	-	4.2	4.4	35	0.2	4.5	13.9	20	3.4
Lab052	5	4.6	4.7	5	0.2	4.3	10.7	20	4.1	4.6	4.7	14	0.2	4.3	10.7	20	4.1
Total	-	-	4.6	15	0.2	4.3	-	-	-	-	4.6	375	0.3	6.5	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE : Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2025 02 Change Cumulative : from 2022 06 01 to 2025 02 28 Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5