Summary Report of IQC program for G6PD Quantitative Test - AMP Group - February 2016 -

I. The statistic results of all laboratories in this month

G6PD	Control N (Lot No.:AC1203N)	Control D (Lot No.:AC1203D)
Labs	9	9
Received results number (n)	44	44
Median	12.7 (U/gHb)	2.9 (U/gHb)
Mean	12.5 (U/gHb)	3.0 (U/gHb)
SD	1.2	0.4
CV	9.6%	13.3%
Range of G6PD	10.5 ~ 16.0 (U/gHb)	2.4 ~ 3.9 (U/gHb)
Range of Hb	2.3 ~ 2.9 (g/dL)	2.5 ~ 3.5 (g/dL)

*The statistic results are calculated from all labs reported in this month

II. The distribution of G6PD reported for each lab in this survey

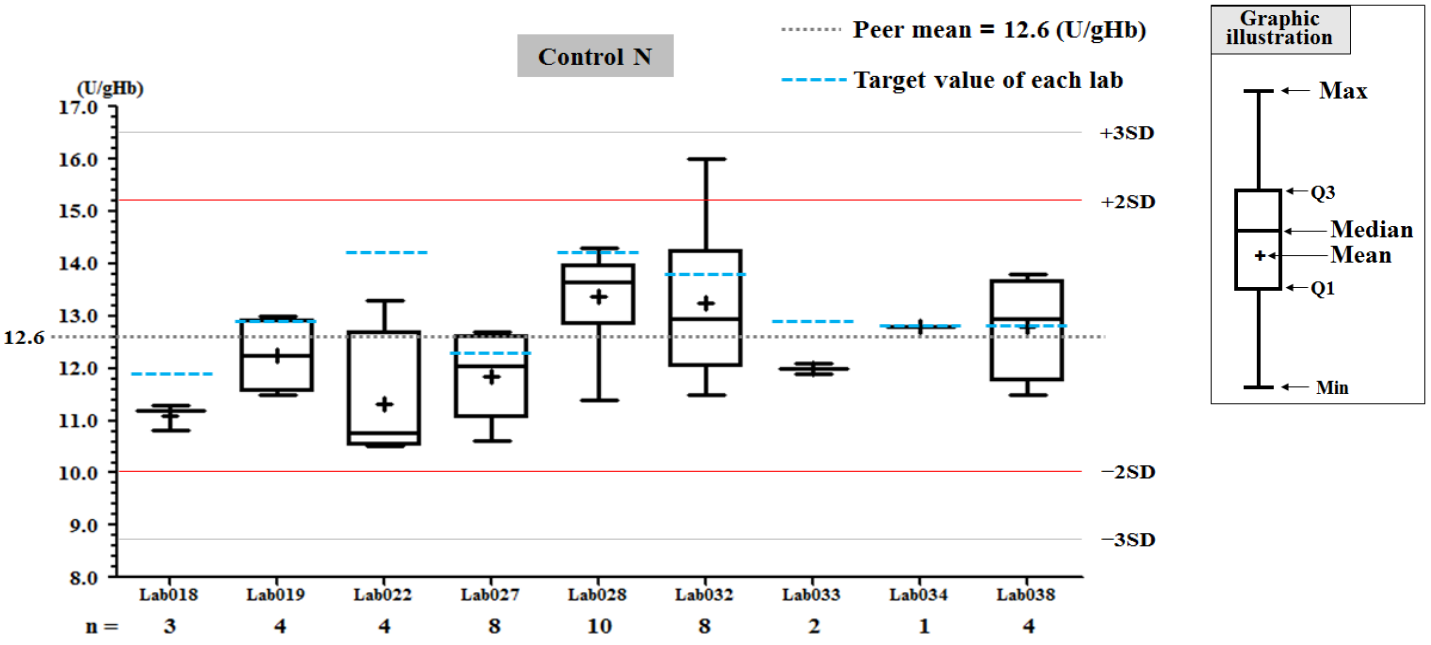

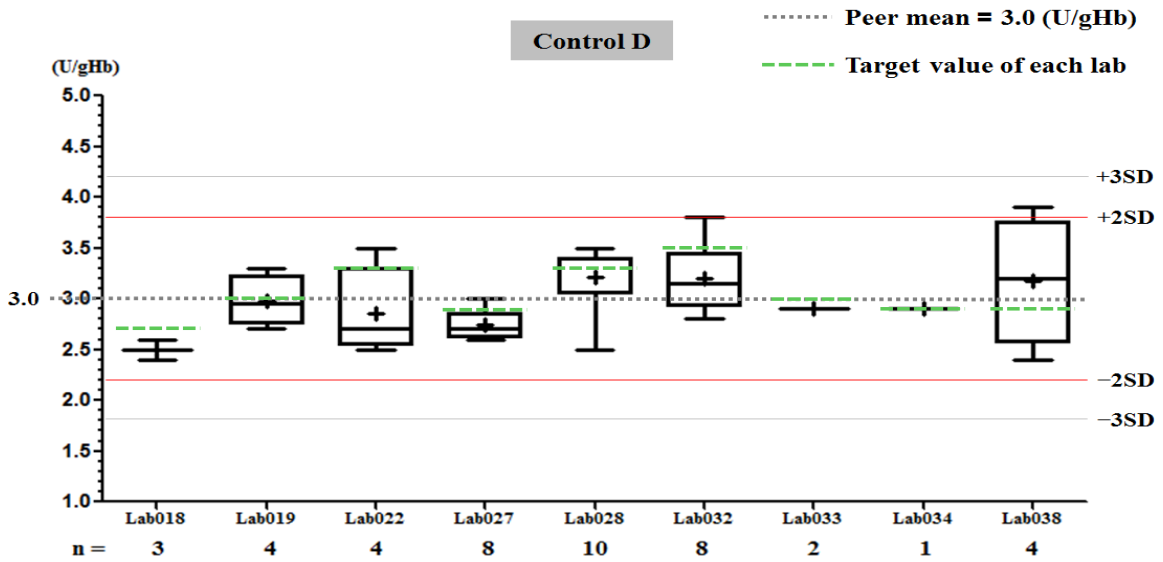

Preventive Medicine Foundation TEL:+886-2-2703-6080 ; FAX:+886-2-2703-6070 ; <g6pd@g6pd.tw> ; <http://iqc.g6pd.tw/>

QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AC1203N (2014-01-01 ~ 2100-12-31) Change

Print Table

Lab022

	Control N		Control D	
QC Control Lot No.	AC1203N		AC1203D	
Duration of the Analyzing	Month (2016/02)	CUM (2014/02/01~2016/02/29)	Month (2016/02)	CUM (2014/02/01~2016/02/29)
Runs (N)	4	22	4	22
Mean (U/gHb)	11.3	11.9	2.9	3.1
SD	1.3	1.1	0.4	0.4
CV (%)	11.5	9.2	13.8	12.9
Target Value (U/gHb)	14.2	14.2	3.3	3.3
Total Error (%)	43.4	34.7	39.7	31.9
TEa (%)	20	20	20	20
σ	0.0	0.4	0.6	1.1

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE : Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2016 02 Change ; Cumulative : from 2014 02 01 to 2016 02 29 Change

[TOP]

Control N SDI QC Chart

Lot No.: AC1203N ; Duration : 2014-02-01 to 2016-02-29 ; Target : 14.2 ; SD : 2.6

Lab022

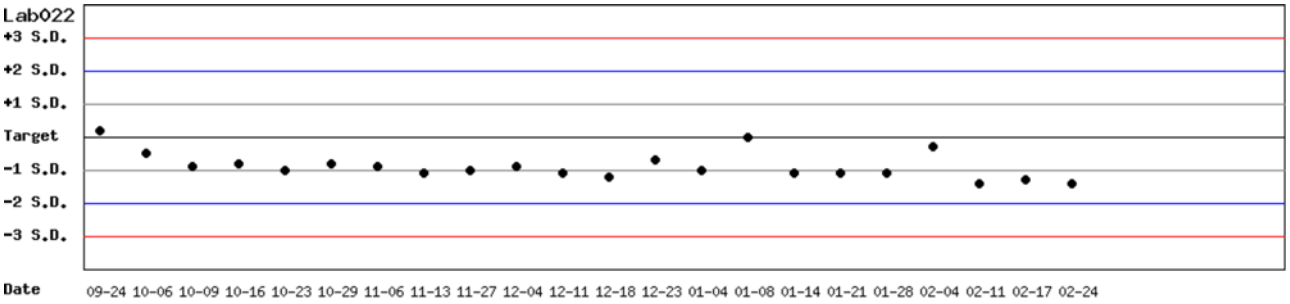

Month : 2016 02 Change ; Cumulative : from 2014 02 01 to 2016 02 29 Change

[TOP]

Control D SDI QC Chart

Lot No.: AC1203D ; Duration : 2014-02-01 to 2016-02-29 ; Target : 3.3 ; SD : 3.1

Lab022

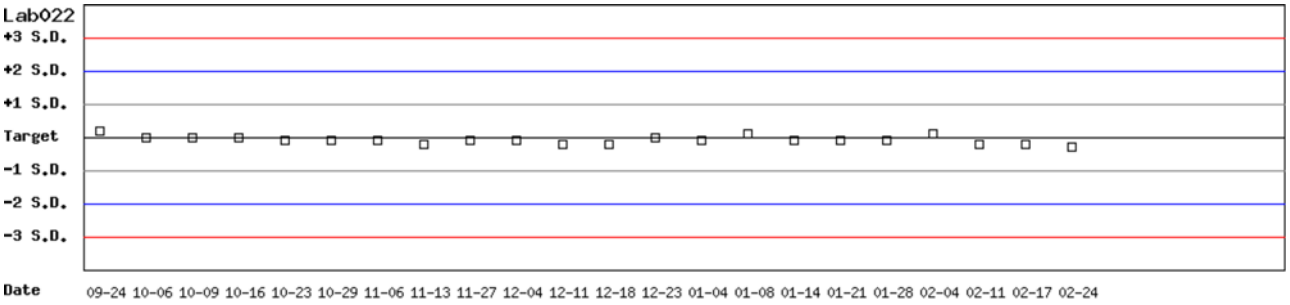

Month : 2016 02 Change ; Cumulative : from 2014 02 01 to 2016 02 29 Change

[TOP]

Control N and **Control D SDI**
QC Chart

Lot No.: AC1203N ; Duration : 2014-02-01 to 2016-02-29 ; Target : 14.2 ; SD : 2.6 (●)

Lot No.: AC1203D ; Duration : 2014-02-01 to 2016-02-29 ; Target : 3.3 ; SD : 3.1 (□)

Lab022

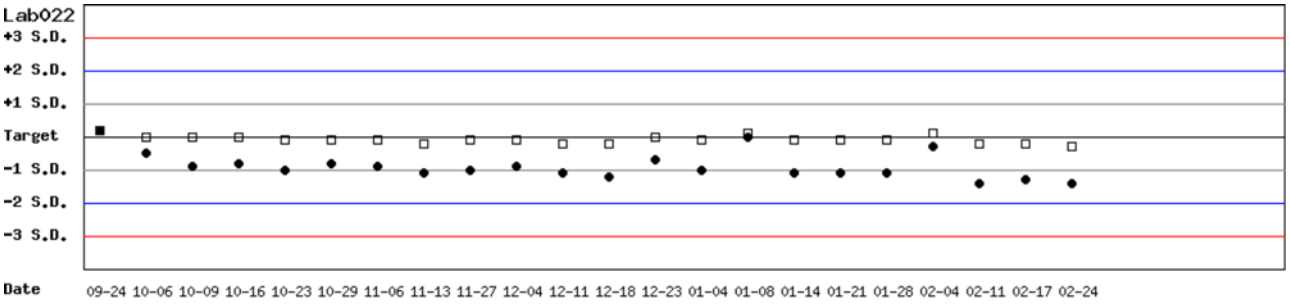

Month : 2016 02 Change ; Cumulative : from 2014 02 01 to 2016 02 29 Change

[TOP]

Peer Group Statistics (Table 1)

Select LotNo：AC1203N (2014-01-01 ~ 2100-12-31) Change

Select Reagent Kit：2 - AMP Change

Print Table 1

Monthly

Month : 2016 02 Change

		Control N (Lot No.: AC1203N)								Control D (Lot No.: AC1203D)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab018	2	11.9	11.1	3	0.3	2.7	12.1	20	4.9	2.7	2.5	3	0.1	4.0	15.4	20	3.1
Lab019	2	12.9	12.3	4	0.7	5.7	16.0	20	2.7	3.0	3.0	4	0.3	10.0	20.0	20	2.0
Lab022	2	14.2	11.3	4	1.3	11.5	43.4	20	0.0	3.3	2.9	4	0.4	13.8	39.7	20	0.6
Lab027	2	12.3	11.9	8	0.8	6.7	16.7	20	2.5	2.9	2.7	8	0.1	3.7	14.3	20	3.5
Lab028	2	14.2	13.4	10	0.9	6.7	19.1	20	2.1	3.3	3.2	10	0.4	12.5	28.0	20	1.4
Lab032	2	13.8	13.3	8	1.5	11.3	26.2	20	1.4	3.5	3.2	8	0.3	9.4	27.3	20	1.2
Lab033	2	12.9	12.0	2	-	-	-	20	-	3.0	2.9	2	-	-	-	20	-
Lab034	2	12.8	12.8	1	-	-	-	20	-	2.9	2.9	1	-	-	-	20	-
Lab038	2	12.8	12.8	4	1.0	7.8	15.6	20	2.6	2.9	3.2	4	0.6	18.8	47.8	20	0.5
Total	-	-	12.5	44	1.2	9.6	-	-	-	-	3.0	44	0.4	13.3	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE：Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[TOP]

Cumulative

Cumulative : from 2014 02 01 to 2016 02 29 Change

		Control N (Lot No.: AC1203N)								Control D (Lot No.: AC1203D)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab017	2	14.2	13.8	36	1.6	11.6	26.0	20	1.5	3.3	3.9	36	1.4	35.9	90.0	20	0.1
Lab018	2	11.9	10.8	75	1.6	14.8	38.9	20	0.7	2.7	2.6	75	1.1	42.3	88.3	20	0.4
Lab019	2	12.9	12.1	104	1.2	9.9	26.0	20	1.4	3.0	2.8	104	0.4	14.3	35.2	20	0.9
Lab021	2	14.2	14.2	54	0.2	1.4	2.8	20	>6	3.3	3.4	54	0.1	2.9	8.9	20	5.9
Lab022	2	14.2	11.9	22	1.1	9.2	34.7	20	0.4	3.3	3.1	22	0.4	12.9	31.9	20	1.1
Lab024	2	11.6	11.1	49	1.2	10.8	25.9	20	1.5	2.7	2.7	49	0.4	14.8	29.6	20	1.4
Lab026	2	11.6	11.5	211	1.6	13.9	28.7	36	2.5	2.7	2.8	211	0.5	17.9	39.4	36	1.8
Lab027	2	12.3	11.8	121	1.6	13.6	31.2	20	1.2	2.9	2.7	121	0.5	18.5	43.9	20	0.7
Lab028	2	14.2	13.9	201	1.2	8.6	19.4	20	2.1	3.3	3.4	201	0.6	17.6	38.3	20	1.0
Lab031	2	12.8	10.1	63	1.4	13.9	48.8	20	-0.1	2.9	2.4	63	0.4	16.7	50.6	20	0.2
Lab032	2	13.8	11.3	175	2.0	17.7	53.5	20	0.1	3.5	2.6	175	0.5	19.2	64.2	20	-0.3
Lab033	2	12.9	12.2	100	1.0	8.2	21.8	20	1.8	3.0	2.9	100	0.3	10.3	24.0	20	1.6
Lab034	2	12.8	12.6	47	0.5	4.0	9.5	20	4.6	2.9	3.0	47	0.1	3.3	10.1	20	5.0
Lab035	2	12.8	12.6	37	0.7	5.6	12.7	20	3.3	2.9	2.9	37	0.3	10.3	20.7	20	1.9
Lab037	2	12.8	12.5	9	1.0	8.0	18.3	20	2.2	2.9	3.1	9	0.3	9.7	26.3	20	1.4
Lab038	2	12.8	12.7	37	1.2	9.4	19.7	20	2.0	2.9	3.2	37	0.5	15.6	41.6	20	0.6
Total	-	-	12.1	1341	1.8	14.9	-	-	-	-	2.9	1341	0.6	20.7	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE：Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[TOP]

Reagent Kit	Reagent Code
AMP	2

Peer Group Statistics (Table 2)

Select LotNo：AC1203N (2014-01-01 ~ 2100-12-31) Change

Select Reagent Kit：2 - AMP Change

Print Table 2

Control N Month vs. Cumulative

		Control N (Lot No.: AC1203N)															
		Month (2016/02)								CUM (2014/02/01~2016/02/29)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab017	2	14.2	-	0	-	-	-	20	-	14.2	13.8	36	1.6	11.6	26.0	20	1.5
Lab018	2	11.9	11.1	3	0.3	2.7	12.1	20	4.9	11.9	10.8	75	1.6	14.8	38.9	20	0.7
Lab019	2	12.9	12.3	4	0.7	5.7	16.0	20	2.7	12.9	12.1	104	1.2	9.9	26.0	20	1.4
Lab021	2	14.2	-	0	-	-	-	20	-	14.2	14.2	54	0.2	1.4	2.8	20	>6
Lab022	2	14.2	11.3	4	1.3	11.5	43.4	20	0.0	14.2	11.9	22	1.1	9.2	34.7	20	0.4
Lab024	2	11.6	-	0	-	-	-	20	-	11.6	11.1	49	1.2	10.8	25.9	20	1.5
Lab026	2	11.6	-	0	-	-	-	36	-	11.6	11.5	211	1.6	13.9	28.7	36	2.5
Lab027	2	12.3	11.9	8	0.8	6.7	16.7	20	2.5	12.3	11.8	121	1.6	13.6	31.2	20	1.2
Lab028	2	14.2	13.4	10	0.9	6.7	19.1	20	2.1	14.2	13.9	201	1.2	8.6	19.4	20	2.1
Lab031	2	12.8	-	0	-	-	-	20	-	12.8	10.1	63	1.4	13.9	48.8	20	-0.1
Lab032	2	13.8	13.3	8	1.5	11.3	26.2	20	1.4	13.8	11.3	175	2.0	17.7	53.5	20	0.1
Lab033	2	12.9	12.0	2	-	-	-	20	-	12.9	12.2	100	1.0	8.2	21.8	20	1.8
Lab034	2	12.8	12.8	1	-	-	-	20	-	12.8	12.6	47	0.5	4.0	9.5	20	4.6
Lab035	2	12.8	-	0	-	-	-	20	-	12.8	12.6	37	0.7	5.6	12.7	20	3.3
Lab037	2	12.8	-	0	-	-	-	20	-	12.8	12.5	9	1.0	8.0	18.3	20	2.2
Lab038	2	12.8	12.8	4	1.0	7.8	15.6	20	2.6	12.8	12.7	37	1.2	9.4	19.7	20	2.0
Total	-	-	12.5	44	1.2	9.6	-	-	-	-	12.1	1341	1.8	14.9	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE：Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2016 02 Change Cumulative : from 2014 02 01 to 2016 02 29 Change

[TOP]

Control D Month vs. Cumulative

		Control D (Lot No.: AC1203D)															
		Month (2016/02)								CUM (2014/02/01~2016/02/29)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab017	2	3.3	-	0	-	-	-	20	-	3.3	3.9	36	1.4	35.9	90.0	20	0.1
Lab018	2	2.7	2.5	3	0.1	4.0	15.4	20	3.1	2.7	2.6	75	1.1	42.3	88.3	20	0.4
Lab019	2	3.0	3.0	4	0.3	10.0	20.0	20	2.0	3.0	2.8	104	0.4	14.3	35.2	20	0.9
Lab021	2	3.3	-	0	-	-	-	20	-	3.3	3.4	54	0.1	2.9	8.9	20	5.9
Lab022	2	3.3	2.9	4	0.4	13.8	39.7	20	0.6	3.3	3.1	22	0.4	12.9	31.9	20	1.1
Lab024	2	2.7	-	0	-	-	-	20	-	2.7	2.7	49	0.4	14.8	29.6	20	1.4
Lab026	2	2.7	-	0	-	-	-	36	-	2.7	2.8	211	0.5	17.9	39.4	36	1.8
Lab027	2	2.9	2.7	8	0.1	3.7	14.3	20	3.5	2.9	2.7	121	0.5	18.5	43.9	20	0.7
Lab028	2	3.3	3.2	10	0.4	12.5	28.0	20	1.4	3.3	3.4	201	0.6	17.6	38.3	20	1.0
Lab031	2	2.9	-	0	-	-	-	20	-	2.9	2.4	63	0.4	16.7	50.6	20	0.2
Lab032	2	3.5	3.2	8	0.3	9.4	27.3	20	1.2	3.5	2.6	175	0.5	19.2	64.2	20	-0.3
Lab033	2	3.0	2.9	2	-	-	-	20	-	3.0	2.9	100	0.3	10.3	24.0	20	1.6
Lab034	2	2.9	2.9	1	-	-	-	20	-	2.9	3.0	47	0.1	3.3	10.1	20	5.0
Lab035	2	2.9	-	0	-	-	-	20	-	2.9	2.9	37	0.3	10.3	20.7	20	1.9
Lab037	2	2.9	-	0	-	-	-	20	-	2.9	3.1	9	0.3	9.7	26.3	20	1.4
Lab038	2	2.9	3.2	4	0.6	18.8	47.8	20	0.5	2.9	3.2	37	0.5	15.6	41.6	20	0.6
Total	-	-	3.0	44	0.4	13.3	-	-	-	-	2.9	1341	0.6	20.7	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE：Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2016 02 Change Cumulative : from 2014 02 01 to 2016 02 29 Change

[TOP]

Reagent Kit	Reagent Code
AMP	2