


# Summary Report of IQC program for G6PD Quantitative Test - AMP Group - September 2016 -

## I. The statistic results of all laboratories in this month

G6PD	Control N (Lot No.:AC1203N)	Control D (Lot No.:AC1203D)
Labs	9	9
Received results number (n)	50	50
Median	12.4 (U/gHb)	3.0 (U/gHb)
Mean	12.2 (U/gHb)	2.9 (U/gHb)
SD	1.1	0.4
CV	9.0%	13.8%
Range of G6PD	9.4 ~ 13.8 (U/gHb)	1.9 ~ 3.5 (U/gHb)
Range of Hb	2.0 ~ 2.8 (g/dL)	2.6 ~ 3.1 (g/dL)

\*The statistic results are calculated from all labs reported in this month

## II. The distribution of G6PD reported for each lab in this survey

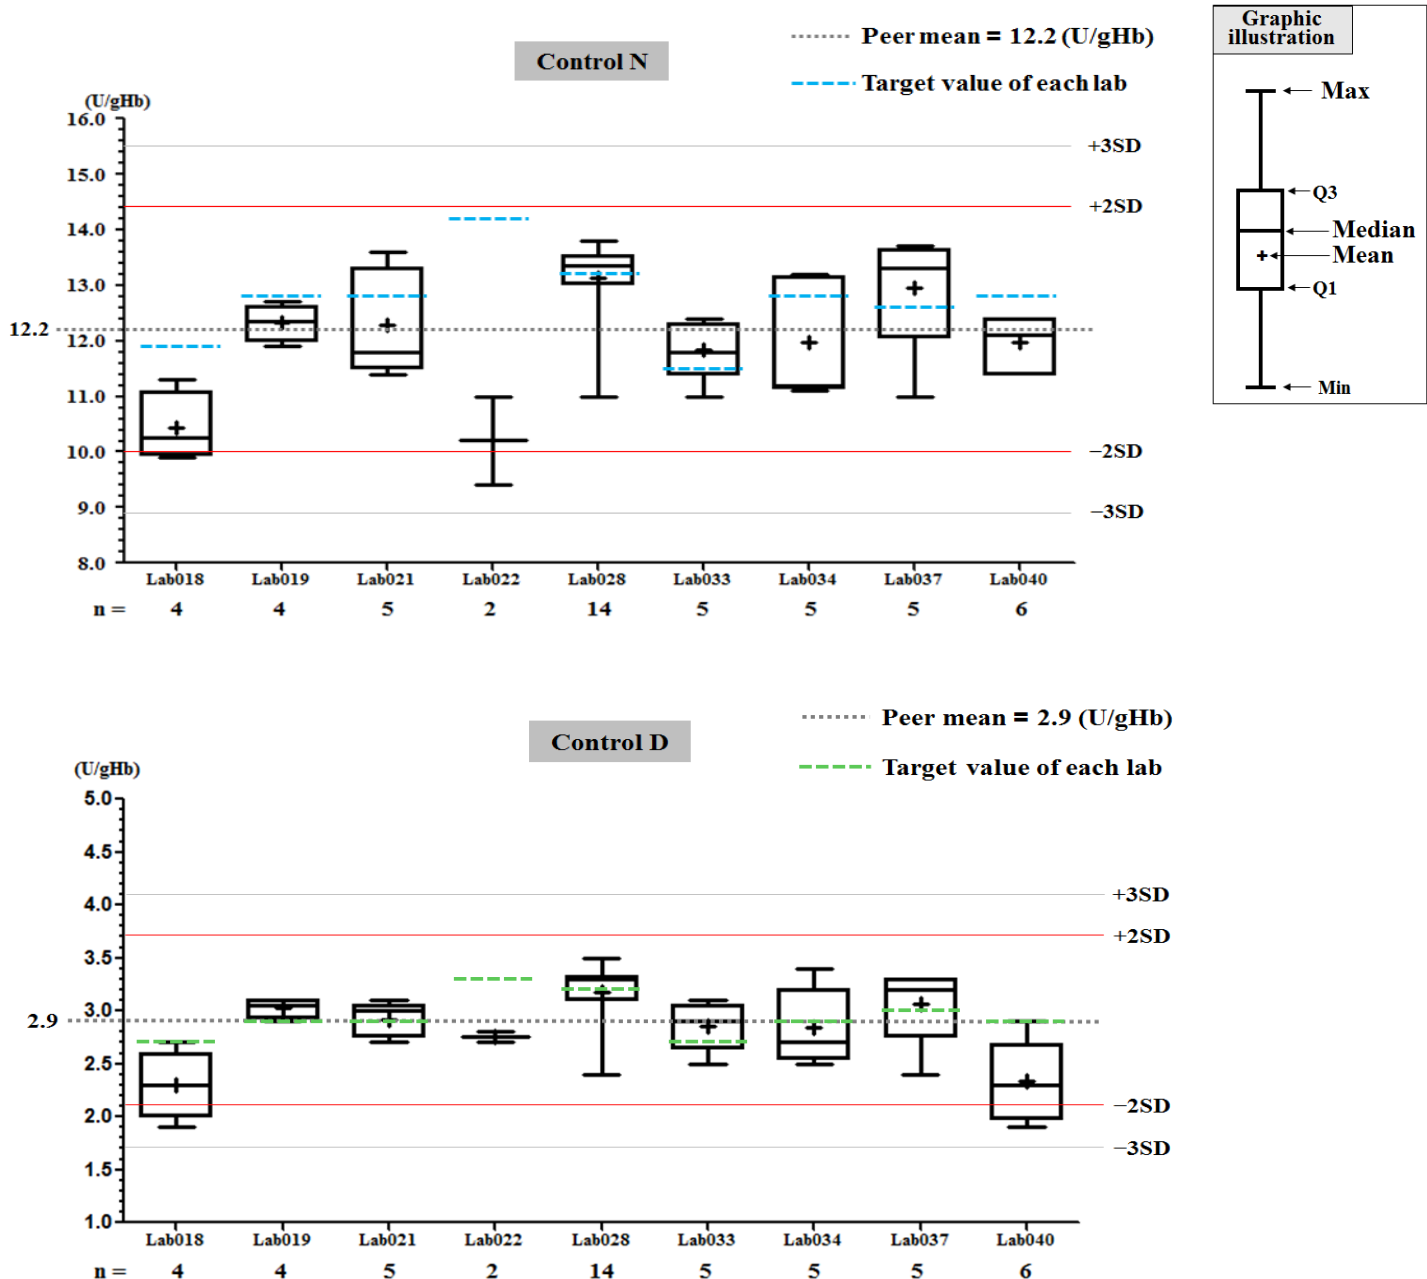

# QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AC1203N (2014-01-01 ~ 2100-12-31) [Change](#)

[Print Table](#)

## Lab021

QC Control Lot No.	Control N		Control D	
	AC1203N		AC1203D	
Duration of the Analyzing	Month (2016/09)	CUM (2016/01/06~2016/09/30)	Month (2016/09)	CUM (2016/01/06~2016/09/30)
Runs (N)	5	26	5	26
Mean (U/gHb)	12.3	12.8	2.9	3.0
SD	1.0	0.9	0.2	0.2
CV (%)	8.1	7.0	6.9	6.7
Target Value (U/gHb)	12.8	12.8	2.9	2.9
Total Error (%)	20.2	14.1	13.8	16.8
TEa (%)	20	20	20	20
$\sigma$	2.0	2.9	2.9	2.5

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 $\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)


Month : 2016 | 09 [Change](#) ; Cumulative : from 2016 | 01 06 to 2016 | 09 30 [Change](#)

[TOP](#)

## Control N SDI QC Chart

Lot No.: AC1203N ; Duration : 2016-01-06 to 2016-09-30 ; Target : 12.8 ; SD : 2.6

Lab021




Month : 2016 | 09 [Change](#) ; Cumulative : from 2016 | 01 06 to 2016 | 09 30 [Change](#)

[TOP](#)

## Control D SDI QC Chart

Lot No.: AC1203D ; Duration : 2016-01-06 to 2016-09-30 ; Target : 2.9 ; SD : 3.1

Lab021



Month : 2016 | 09 [Change](#) ; Cumulative : from 2016 | 01 06 to 2016 | 09 30 [Change](#)


[TOP](#)

**Control N and Control D SDI  
QC Chart**

Lot No.: AC1203N ; Duration : 2016-01-06 to 2016-09-30 ; Target : 12.8 ; SD : 2.6 ( ● )

Lot No.: AC1203D ; Duration : 2016-01-06 to 2016-09-30 ; Target : 2.9 ; SD : 3.1 ( □ )

Lab021



Month : 2016 | 09  ; Cumulative : from 2016 | 01 06 to 2016 | 09 30

[TOP](#)

# Peer Group Statistics (Table 1)

Select LotNo :

Select Reagent Kit :

## Monthly

Month :

UnitID ↑	Reagent Kit (Code) ↑	Control N (Lot No.: AC1203N)								Control D (Lot No.: AC1203D)							
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	2	11.9	10.4	4	0.6	5.8	24.1	20	1.3	2.7	2.3	4	0.3	13.0	40.9	20	0.4
<a href="#">Lab019</a>	2	12.8	12.3	4	0.3	2.4	8.8	20	>6	2.9	3.0	4	0.1	3.3	10.1	20	5.0
<a href="#">Lab021</a>	2	12.8	12.3	5	1.0	8.1	20.2	20	2.0	2.9	2.9	5	0.2	6.9	13.8	20	2.9
<a href="#">Lab022</a>	2	14.2	10.2	2	-	-	-	20	-	3.3	2.8	2	-	-	-	20	-
<a href="#">Lab028</a>	2	13.2	13.1	14	0.7	5.3	11.4	20	3.6	3.2	3.2	14	0.3	9.4	18.8	20	2.1
<a href="#">Lab033</a>	2	11.5	11.8	5	0.5	4.2	11.1	20	4.1	2.7	2.9	5	0.2	6.9	21.2	20	1.8
<a href="#">Lab034</a>	2	12.8	12.0	5	1.1	9.2	24.6	20	1.5	2.9	2.8	5	0.4	14.3	32.0	20	1.2
<a href="#">Lab037</a>	2	12.6	12.9	5	1.1	8.5	19.4	20	2.1	3.0	3.1	5	0.4	12.9	29.1	20	1.3
<a href="#">Lab040</a>	2	12.8	12.0	6	0.5	4.2	14.6	20	3.3	2.9	2.3	6	0.4	17.4	55.5	20	0.0
Total	-	-	12.2	50	1.1	9.0	-	-	-	-	2.9	50	0.4	13.8	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

## Cumulative

Cumulative : from    to

UnitID ↑	Reagent Kit (Code) ↑	Control N (Lot No.: AC1203N)								Control D (Lot No.: AC1203D)							
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab017</a>	2	14.2	13.8	36	1.6	11.6	26.0	20	1.5	3.3	3.9	36	1.4	35.9	90.0	20	0.1
<a href="#">Lab018</a>	2	11.9	10.9	105	1.4	12.8	34.1	20	0.9	2.7	2.6	105	0.9	34.6	72.9	20	0.5
<a href="#">Lab019</a>	2	12.8	12.2	136	1.2	9.8	24.4	20	1.6	2.9	2.8	136	0.4	14.3	32.0	20	1.2
<a href="#">Lab021</a>	2	12.8	13.7	76	0.9	6.6	20.2	20	2.0	2.9	3.3	76	0.3	9.1	32.0	20	0.7
<a href="#">Lab022</a>	2	14.2	11.5	57	1.2	10.4	39.9	20	0.1	3.3	2.9	57	0.3	10.3	32.8	20	0.8
<a href="#">Lab024</a>	2	11.6	11.1	58	1.2	10.8	25.9	20	1.5	2.7	2.7	58	0.3	11.1	22.2	20	1.8
<a href="#">Lab026</a>	2	11.6	11.5	212	1.6	13.9	28.7	36	2.5	2.7	2.8	212	0.5	17.9	39.4	36	1.8
<a href="#">Lab027</a>	2	12.3	11.8	147	1.6	13.6	31.2	20	1.2	2.9	2.7	147	0.5	18.5	43.9	20	0.7
<a href="#">Lab028</a>	2	13.2	13.7	296	1.2	8.8	21.3	20	1.8	3.2	3.3	296	0.5	15.2	33.4	20	1.1
<a href="#">Lab031</a>	2	12.8	10.4	89	1.5	14.4	47.6	20	0.1	2.9	2.5	89	0.5	20.0	53.8	20	0.3
<a href="#">Lab032</a>	2	12.3	11.5	222	1.9	16.5	39.5	20	0.8	2.9	2.7	222	0.5	18.5	43.9	20	0.7
<a href="#">Lab033</a>	2	11.5	12.0	125	1.0	8.3	21.0	20	1.9	2.7	2.9	125	0.3	10.3	28.1	20	1.2
<a href="#">Lab034</a>	2	12.8	12.4	73	0.7	5.6	14.4	20	3.0	2.9	3.0	73	0.2	6.7	16.8	20	2.5
<a href="#">Lab035</a>	2	12.8	12.4	55	0.7	5.6	14.4	20	3.0	2.9	2.8	55	0.3	10.7	24.9	20	1.5
<a href="#">Lab037</a>	2	12.6	12.7	40	1.2	9.4	19.7	20	2.0	3.0	3.0	40	0.4	13.3	26.7	20	1.5
<a href="#">Lab038</a>	2	12.8	12.7	55	1.0	7.9	16.5	20	2.4	2.9	3.1	55	0.5	16.1	39.2	20	0.8
<a href="#">Lab040</a>	2	12.8	11.8	11	0.5	4.2	16.3	20	2.9	2.9	2.4	11	0.3	12.5	42.2	20	0.2
Total	-	-	12.1	1793	1.7	14.0	-	-	-	-	2.9	1793	0.6	20.7	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

Reagent Kit	Reagent Code
AMP	2

## Peer Group Statistics (Table 2)

Select LotNo :

Select Reagent Kit :

### Control N Month vs. Cumulative

		Control N (Lot No.: AC1203N)															
		Month (2016/09)									CUM (2014/02/01~2016/09/30)						
UnitID <sup>⬇</sup>	Reagent Kit (Code) <sup>⬇</sup>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab017</a>	2	14.2	-	0	-	-	-	20	-	14.2	13.8	36	1.6	11.6	26.0	20	1.5
<a href="#">Lab018</a>	2	11.9	10.4	4	0.6	5.8	24.1	20	1.3	11.9	10.9	105	1.4	12.8	34.1	20	0.9
<a href="#">Lab019</a>	2	12.8	12.3	4	0.3	2.4	8.8	20	>6	12.8	12.2	136	1.2	9.8	24.4	20	1.6
<a href="#">Lab021</a>	2	12.8	12.3	5	1.0	8.1	20.2	20	2.0	12.8	13.7	76	0.9	6.6	20.2	20	2.0
<a href="#">Lab022</a>	2	14.2	10.2	2	-	-	-	20	-	14.2	11.5	57	1.2	10.4	39.9	20	0.1
<a href="#">Lab024</a>	2	11.6	-	0	-	-	-	20	-	11.6	11.1	58	1.2	10.8	25.9	20	1.5
<a href="#">Lab026</a>	2	11.6	-	0	-	-	-	36	-	11.6	11.5	212	1.6	13.9	28.7	36	2.5
<a href="#">Lab027</a>	2	12.3	-	0	-	-	-	20	-	12.3	11.8	147	1.6	13.6	31.2	20	1.2
<a href="#">Lab028</a>	2	13.2	13.1	14	0.7	5.3	11.4	20	3.6	13.2	13.7	296	1.2	8.8	21.3	20	1.8
<a href="#">Lab031</a>	2	12.8	-	0	-	-	-	20	-	12.8	10.4	89	1.5	14.4	47.6	20	0.1
<a href="#">Lab032</a>	2	12.3	-	0	-	-	-	20	-	12.3	11.5	222	1.9	16.5	39.5	20	0.8
<a href="#">Lab033</a>	2	11.5	11.8	5	0.5	4.2	11.1	20	4.1	11.5	12.0	125	1.0	8.3	21.0	20	1.9
<a href="#">Lab034</a>	2	12.8	12.0	5	1.1	9.2	24.6	20	1.5	12.8	12.4	73	0.7	5.6	14.4	20	3.0
<a href="#">Lab035</a>	2	12.8	-	0	-	-	-	20	-	12.8	12.4	55	0.7	5.6	14.4	20	3.0
<a href="#">Lab037</a>	2	12.6	12.9	5	1.1	8.5	19.4	20	2.1	12.6	12.7	40	1.2	9.4	19.7	20	2.0
<a href="#">Lab038</a>	2	12.8	-	0	-	-	-	20	-	12.8	12.7	55	1.0	7.9	16.5	20	2.4
<a href="#">Lab040</a>	2	12.8	12.0	6	0.5	4.2	14.6	20	3.3	12.8	11.8	11	0.5	4.2	16.3	20	2.9
<b>Total</b>	-	-	12.2	50	1.1	9.0	-	-	-	-	12.1	1793	1.7	14.0	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month :

Cumulative : from    to

[TOP](#)

### Control D Month vs. Cumulative

		Control D (Lot No.: AC1203D)															
		Month (2016/09)									CUM (2014/02/01~2016/09/30)						
UnitID <sup>⬇</sup>	Reagent Kit (Code) <sup>⬇</sup>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab017</a>	2	3.3	-	0	-	-	-	20	-	3.3	3.9	36	1.4	35.9	90.0	20	0.1
<a href="#">Lab018</a>	2	2.7	2.3	4	0.3	13.0	40.9	20	0.4	2.7	2.6	105	0.9	34.6	72.9	20	0.5
<a href="#">Lab019</a>	2	2.9	3.0	4	0.1	3.3	10.1	20	5.0	2.9	2.8	136	0.4	14.3	32.0	20	1.2
<a href="#">Lab021</a>	2	2.9	2.9	5	0.2	6.9	13.8	20	2.9	2.9	3.3	76	0.3	9.1	32.0	20	0.7
<a href="#">Lab022</a>	2	3.3	2.8	2	-	-	-	20	-	3.3	2.9	57	0.3	10.3	32.8	20	0.8
<a href="#">Lab024</a>	2	2.7	-	0	-	-	-	20	-	2.7	2.7	58	0.3	11.1	22.2	20	1.8
<a href="#">Lab026</a>	2	2.7	-	0	-	-	-	36	-	2.7	2.8	212	0.5	17.9	39.4	36	1.8
<a href="#">Lab027</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.7	147	0.5	18.5	43.9	20	0.7
<a href="#">Lab028</a>	2	3.2	3.2	14	0.3	9.4	18.8	20	2.1	3.2	3.3	296	0.5	15.2	33.4	20	1.1
<a href="#">Lab031</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.5	89	0.5	20.0	53.8	20	0.3
<a href="#">Lab032</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.7	222	0.5	18.5	43.9	20	0.7
<a href="#">Lab033</a>	2	2.7	2.9	5	0.2	6.9	21.2	20	1.8	2.7	2.9	125	0.3	10.3	28.1	20	1.2
<a href="#">Lab034</a>	2	2.9	2.8	5	0.4	14.3	32.0	20	1.2	2.9	3.0	73	0.2	6.7	16.8	20	2.5
<a href="#">Lab035</a>	2	2.9	-	0	-	-	-	20	-	2.9	2.8	55	0.3	10.7	24.9	20	1.5
<a href="#">Lab037</a>	2	3.0	3.1	5	0.4	12.9	29.1	20	1.3	3.0	3.0	40	0.4	13.3	26.7	20	1.5
<a href="#">Lab038</a>	2	2.9	-	0	-	-	-	20	-	2.9	3.1	55	0.5	16.1	39.2	20	0.8
<a href="#">Lab040</a>	2	2.9	2.3	6	0.4	17.4	55.5	20	0.0	2.9	2.4	11	0.3	12.5	42.2	20	0.2
<b>Total</b>	-	-	2.9	50	0.4	13.8	-	-	-	-	2.9	1793	0.6	20.7	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month :

Cumulative : from    to

[TOP](#)

Reagent Kit	Reagent Code
AMP	2