


# Summary Report of IQC program for G6PD Quantitative Test - AMP Group - September 2016 -

## I. The statistic results of all laboratories in this month

| G6PD                        | Control N<br>(Lot No.:AC1203N) | Control D<br>(Lot No.:AC1203D) |
|-----------------------------|--------------------------------|--------------------------------|
| Labs                        | 9                              | 9                              |
| Received results number (n) | 50                             | 50                             |
| Median                      | 12.4 (U/gHb)                   | 3.0 (U/gHb)                    |
| Mean                        | 12.2 (U/gHb)                   | 2.9 (U/gHb)                    |
| SD                          | 1.1                            | 0.4                            |
| CV                          | 9.0%                           | 13.8%                          |
| Range of G6PD               | 9.4 ~ 13.8 (U/gHb)             | 1.9 ~ 3.5 (U/gHb)              |
| Range of Hb                 | 2.0 ~ 2.8 (g/dL)               | 2.6 ~ 3.1 (g/dL)               |

\*The statistic results are calculated from all labs reported in this month

## II. The distribution of G6PD reported for each lab in this survey

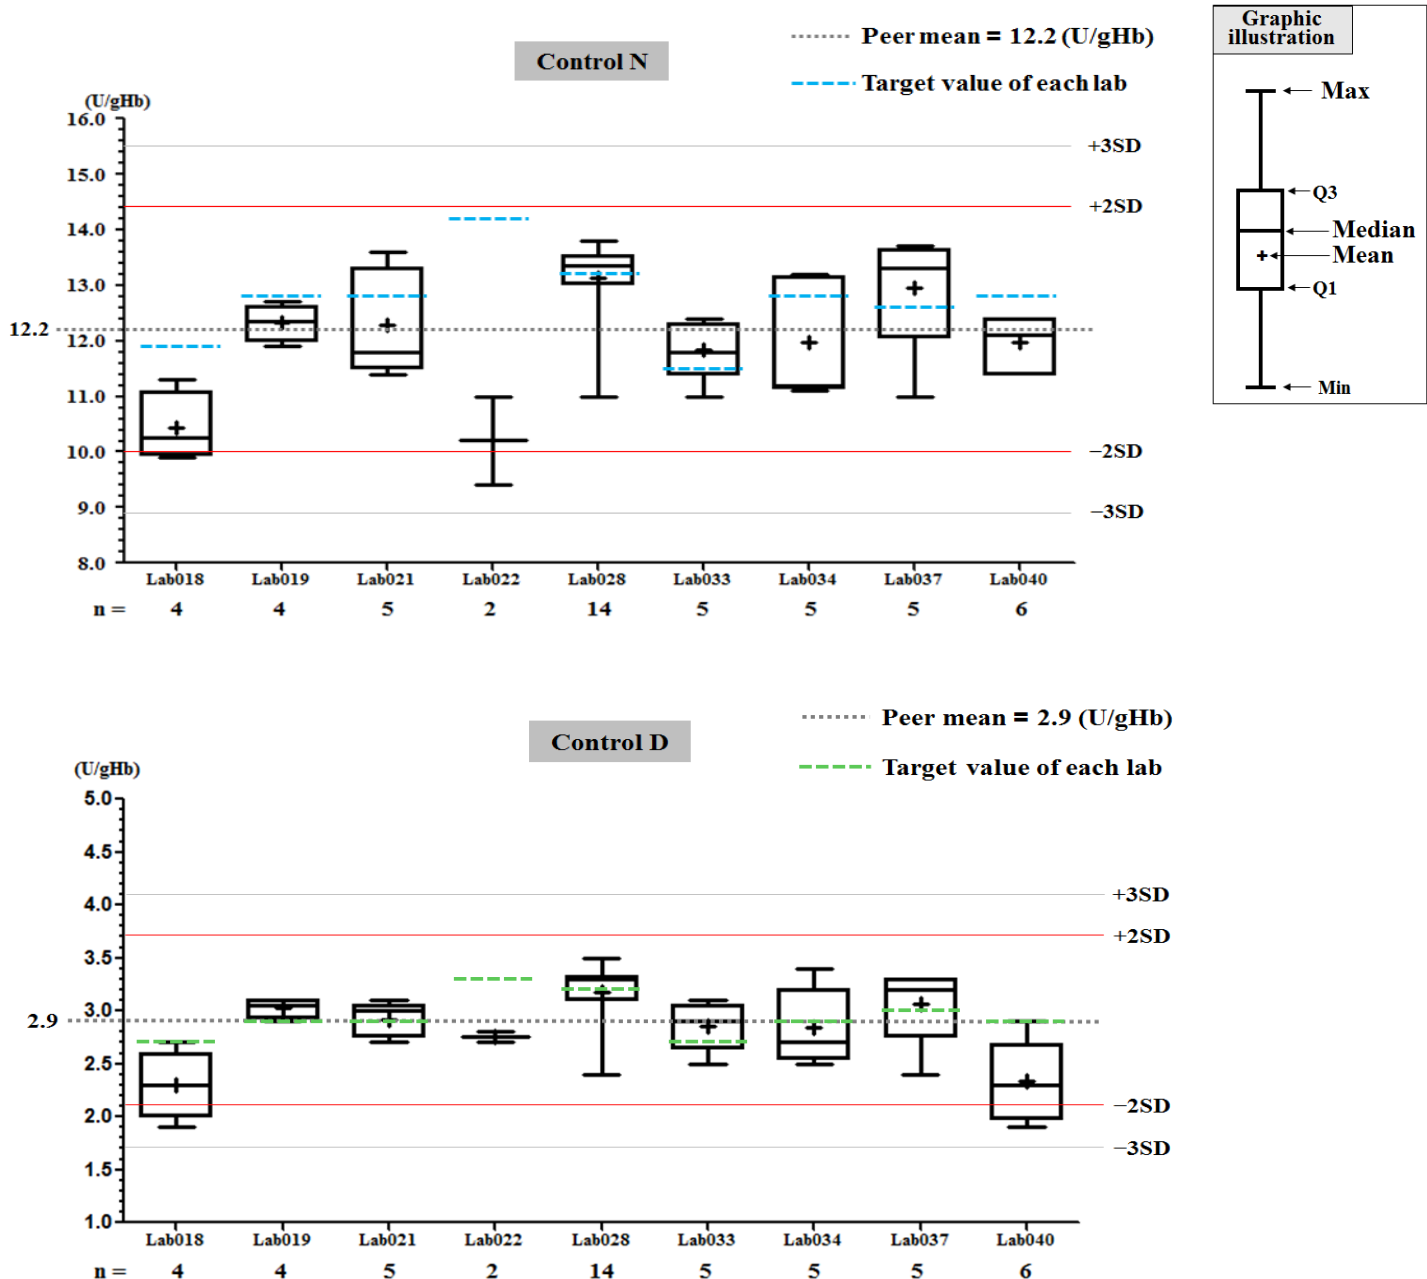

# QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AC1203N (2014-01-01 ~ 2100-12-31) [Change](#)

[Print Table](#)

## Lab033

| QC Control Lot No.        | Control N       |                             | Control D       |                             |
|---------------------------|-----------------|-----------------------------|-----------------|-----------------------------|
|                           | AC1203N         |                             | AC1203D         |                             |
| Duration of the Analyzing | Month (2016/09) | CUM (2016/01/28~2016/09/30) | Month (2016/09) | CUM (2016/01/28~2016/09/30) |
| Runs (N)                  | 5               | 25                          | 5               | 25                          |
| Mean (U/gHb)              | 11.8            | 11.5                        | 2.9             | 2.8                         |
| SD                        | 0.5             | 0.7                         | 0.2             | 0.3                         |
| CV (%)                    | 4.2             | 6.1                         | 6.9             | 10.7                        |
| Target Value (U/gHb)      | 11.5            | 11.5                        | 2.7             | 2.7                         |
| Total Error (%)           | 11.1            | 12.2                        | 21.2            | 25.1                        |
| TEa (%)                   | 20              | 20                          | 20              | 20                          |
| $\sigma$                  | 4.1             | 3.3                         | 1.8             | 1.5                         |

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 $\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)


Month : 2016 | 09 [Change](#) ; Cumulative : from 2016 | 01 28 to 2016 | 09 30 [Change](#)

[TOP](#)

## Control N SDI QC Chart

Lot No.: AC1203N ; Duration : 2016-01-28 to 2016-09-30 ; Target : 11.5 ; SD : 1.00

Lab033




Month : 2016 | 09 [Change](#) ; Cumulative : from 2016 | 01 28 to 2016 | 09 30 [Change](#)

[TOP](#)

## Control D SDI QC Chart

Lot No.: AC1203D ; Duration : 2016-01-28 to 2016-09-30 ; Target : 2.7 ; SD : 0.30

Lab033



Month : 2016 | 09 [Change](#) ; Cumulative : from 2016 | 01 28 to 2016 | 09 30 [Change](#)


[TOP](#)

## Control N and Control D SDI QC Chart

Lot No.: AC1203N ; Duration : 2016-01-28 to 2016-09-30 ; Target : 11.5 ; SD : 1.00 ( ● )

Lot No.: AC1203D ; Duration : 2016-01-28 to 2016-09-30 ; Target : 2.7 ; SD : 0.30 ( ◻ )

Lab033



Date 01-28 01-28 02-04 02-11 05-12 05-19 05-26 06-02 06-09 06-16 06-23 06-30 07-07 07-14 07-21 07-28 08-04 08-11 08-18 08-25 09-01 09-08 09-15 09-22 09-29

Month : 2016 | 09  ; Cumulative : from 2016 | 01 28 to 2016 | 09 30

[TOP](#)

# Peer Group Statistics (Table 1)

Select LotNo :

Select Reagent Kit :

## Monthly

Month :

| UnitID <sup>↑</sup>    | Reagent Kit (Code) <sup>↑</sup> | Control N (Lot No.: AC1203N) |              |            |     |        |        |         |     | Control D (Lot No.: AC1203D) |              |            |     |        |        |         |     |
|------------------------|---------------------------------|------------------------------|--------------|------------|-----|--------|--------|---------|-----|------------------------------|--------------|------------|-----|--------|--------|---------|-----|
|                        |                                 | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   |
| <a href="#">Lab018</a> | 2                               | 11.9                         | 10.4         | 4          | 0.6 | 5.8    | 24.1   | 20      | 1.3 | 2.7                          | 2.3          | 4          | 0.3 | 13.0   | 40.9   | 20      | 0.4 |
| <a href="#">Lab019</a> | 2                               | 12.8                         | 12.3         | 4          | 0.3 | 2.4    | 8.8    | 20      | >6  | 2.9                          | 3.0          | 4          | 0.1 | 3.3    | 10.1   | 20      | 5.0 |
| <a href="#">Lab021</a> | 2                               | 12.8                         | 12.3         | 5          | 1.0 | 8.1    | 20.2   | 20      | 2.0 | 2.9                          | 2.9          | 5          | 0.2 | 6.9    | 13.8   | 20      | 2.9 |
| <a href="#">Lab022</a> | 2                               | 14.2                         | 10.2         | 2          | -   | -      | -      | 20      | -   | 3.3                          | 2.8          | 2          | -   | -      | -      | 20      | -   |
| <a href="#">Lab028</a> | 2                               | 13.2                         | 13.1         | 14         | 0.7 | 5.3    | 11.4   | 20      | 3.6 | 3.2                          | 3.2          | 14         | 0.3 | 9.4    | 18.8   | 20      | 2.1 |
| <a href="#">Lab033</a> | 2                               | 11.5                         | 11.8         | 5          | 0.5 | 4.2    | 11.1   | 20      | 4.1 | 2.7                          | 2.9          | 5          | 0.2 | 6.9    | 21.2   | 20      | 1.8 |
| <a href="#">Lab034</a> | 2                               | 12.8                         | 12.0         | 5          | 1.1 | 9.2    | 24.6   | 20      | 1.5 | 2.9                          | 2.8          | 5          | 0.4 | 14.3   | 32.0   | 20      | 1.2 |
| <a href="#">Lab037</a> | 2                               | 12.6                         | 12.9         | 5          | 1.1 | 8.5    | 19.4   | 20      | 2.1 | 3.0                          | 3.1          | 5          | 0.4 | 12.9   | 29.1   | 20      | 1.3 |
| <a href="#">Lab040</a> | 2                               | 12.8                         | 12.0         | 6          | 0.5 | 4.2    | 14.6   | 20      | 3.3 | 2.9                          | 2.3          | 6          | 0.4 | 17.4   | 55.5   | 20      | 0.0 |
| <b>Total</b>           | -                               | -                            | 12.2         | 50         | 1.1 | 9.0    | -      | -       | -   | -                            | 2.9          | 50         | 0.4 | 13.8   | -      | -       | -   |

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

## Cumulative

Cumulative : from    to

| UnitID <sup>↑</sup>    | Reagent Kit (Code) <sup>↑</sup> | Control N (Lot No.: AC1203N) |              |            |     |        |        |         |     | Control D (Lot No.: AC1203D) |              |            |     |        |        |         |     |
|------------------------|---------------------------------|------------------------------|--------------|------------|-----|--------|--------|---------|-----|------------------------------|--------------|------------|-----|--------|--------|---------|-----|
|                        |                                 | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   |
| <a href="#">Lab017</a> | 2                               | 14.2                         | 13.8         | 36         | 1.6 | 11.6   | 26.0   | 20      | 1.5 | 3.3                          | 3.9          | 36         | 1.4 | 35.9   | 90.0   | 20      | 0.1 |
| <a href="#">Lab018</a> | 2                               | 11.9                         | 10.9         | 105        | 1.4 | 12.8   | 34.1   | 20      | 0.9 | 2.7                          | 2.6          | 105        | 0.9 | 34.6   | 72.9   | 20      | 0.5 |
| <a href="#">Lab019</a> | 2                               | 12.8                         | 12.2         | 136        | 1.2 | 9.8    | 24.4   | 20      | 1.6 | 2.9                          | 2.8          | 136        | 0.4 | 14.3   | 32.0   | 20      | 1.2 |
| <a href="#">Lab021</a> | 2                               | 12.8                         | 13.7         | 76         | 0.9 | 6.6    | 20.2   | 20      | 2.0 | 2.9                          | 3.3          | 76         | 0.3 | 9.1    | 32.0   | 20      | 0.7 |
| <a href="#">Lab022</a> | 2                               | 14.2                         | 11.5         | 57         | 1.2 | 10.4   | 39.9   | 20      | 0.1 | 3.3                          | 2.9          | 57         | 0.3 | 10.3   | 32.8   | 20      | 0.8 |
| <a href="#">Lab024</a> | 2                               | 11.6                         | 11.1         | 58         | 1.2 | 10.8   | 25.9   | 20      | 1.5 | 2.7                          | 2.7          | 58         | 0.3 | 11.1   | 22.2   | 20      | 1.8 |
| <a href="#">Lab026</a> | 2                               | 11.6                         | 11.5         | 212        | 1.6 | 13.9   | 28.7   | 36      | 2.5 | 2.7                          | 2.8          | 212        | 0.5 | 17.9   | 39.4   | 36      | 1.8 |
| <a href="#">Lab027</a> | 2                               | 12.3                         | 11.8         | 147        | 1.6 | 13.6   | 31.2   | 20      | 1.2 | 2.9                          | 2.7          | 147        | 0.5 | 18.5   | 43.9   | 20      | 0.7 |
| <a href="#">Lab028</a> | 2                               | 13.2                         | 13.7         | 296        | 1.2 | 8.8    | 21.3   | 20      | 1.8 | 3.2                          | 3.3          | 296        | 0.5 | 15.2   | 33.4   | 20      | 1.1 |
| <a href="#">Lab031</a> | 2                               | 12.8                         | 10.4         | 89         | 1.5 | 14.4   | 47.6   | 20      | 0.1 | 2.9                          | 2.5          | 89         | 0.5 | 20.0   | 53.8   | 20      | 0.3 |
| <a href="#">Lab032</a> | 2                               | 12.3                         | 11.5         | 222        | 1.9 | 16.5   | 39.5   | 20      | 0.8 | 2.9                          | 2.7          | 222        | 0.5 | 18.5   | 43.9   | 20      | 0.7 |
| <a href="#">Lab033</a> | 2                               | 11.5                         | 12.0         | 125        | 1.0 | 8.3    | 21.0   | 20      | 1.9 | 2.7                          | 2.9          | 125        | 0.3 | 10.3   | 28.1   | 20      | 1.2 |
| <a href="#">Lab034</a> | 2                               | 12.8                         | 12.4         | 73         | 0.7 | 5.6    | 14.4   | 20      | 3.0 | 2.9                          | 3.0          | 73         | 0.2 | 6.7    | 16.8   | 20      | 2.5 |
| <a href="#">Lab035</a> | 2                               | 12.8                         | 12.4         | 55         | 0.7 | 5.6    | 14.4   | 20      | 3.0 | 2.9                          | 2.8          | 55         | 0.3 | 10.7   | 24.9   | 20      | 1.5 |
| <a href="#">Lab037</a> | 2                               | 12.6                         | 12.7         | 40         | 1.2 | 9.4    | 19.7   | 20      | 2.0 | 3.0                          | 3.0          | 40         | 0.4 | 13.3   | 26.7   | 20      | 1.5 |
| <a href="#">Lab038</a> | 2                               | 12.8                         | 12.7         | 55         | 1.0 | 7.9    | 16.5   | 20      | 2.4 | 2.9                          | 3.1          | 55         | 0.5 | 16.1   | 39.2   | 20      | 0.8 |
| <a href="#">Lab040</a> | 2                               | 12.8                         | 11.8         | 11         | 0.5 | 4.2    | 16.3   | 20      | 2.9 | 2.9                          | 2.4          | 11         | 0.3 | 12.5   | 42.2   | 20      | 0.2 |
| <b>Total</b>           | -                               | -                            | 12.1         | 1793       | 1.7 | 14.0   | -      | -       | -   | -                            | 2.9          | 1793       | 0.6 | 20.7   | -      | -       | -   |

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

| Reagent Kit | Reagent Code |
|-------------|--------------|
| AMP         | 2            |

## Peer Group Statistics (Table 2)

Select LotNo :

Select Reagent Kit :

### Control N Month vs. Cumulative

|                        |                                 | Control N (Lot No.: AC1203N) |              |            |     |        |        |         |     |                |                             |            |     |        |        |         |     |
|------------------------|---------------------------------|------------------------------|--------------|------------|-----|--------|--------|---------|-----|----------------|-----------------------------|------------|-----|--------|--------|---------|-----|
|                        |                                 | Month (2016/09)              |              |            |     |        |        |         |     |                | CUM (2014/02/01~2016/09/30) |            |     |        |        |         |     |
| UnitID <sup>⬇</sup>    | Reagent Kit (Code) <sup>⬇</sup> | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   | Target (U/gHb) | Mean (U/gHb)                | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   |
| <a href="#">Lab017</a> | 2                               | 14.2                         | -            | 0          | -   | -      | -      | 20      | -   | 14.2           | 13.8                        | 36         | 1.6 | 11.6   | 26.0   | 20      | 1.5 |
| <a href="#">Lab018</a> | 2                               | 11.9                         | 10.4         | 4          | 0.6 | 5.8    | 24.1   | 20      | 1.3 | 11.9           | 10.9                        | 105        | 1.4 | 12.8   | 34.1   | 20      | 0.9 |
| <a href="#">Lab019</a> | 2                               | 12.8                         | 12.3         | 4          | 0.3 | 2.4    | 8.8    | 20      | >6  | 12.8           | 12.2                        | 136        | 1.2 | 9.8    | 24.4   | 20      | 1.6 |
| <a href="#">Lab021</a> | 2                               | 12.8                         | 12.3         | 5          | 1.0 | 8.1    | 20.2   | 20      | 2.0 | 12.8           | 13.7                        | 76         | 0.9 | 6.6    | 20.2   | 20      | 2.0 |
| <a href="#">Lab022</a> | 2                               | 14.2                         | 10.2         | 2          | -   | -      | -      | 20      | -   | 14.2           | 11.5                        | 57         | 1.2 | 10.4   | 39.9   | 20      | 0.1 |
| <a href="#">Lab024</a> | 2                               | 11.6                         | -            | 0          | -   | -      | -      | 20      | -   | 11.6           | 11.1                        | 58         | 1.2 | 10.8   | 25.9   | 20      | 1.5 |
| <a href="#">Lab026</a> | 2                               | 11.6                         | -            | 0          | -   | -      | -      | 36      | -   | 11.6           | 11.5                        | 212        | 1.6 | 13.9   | 28.7   | 36      | 2.5 |
| <a href="#">Lab027</a> | 2                               | 12.3                         | -            | 0          | -   | -      | -      | 20      | -   | 12.3           | 11.8                        | 147        | 1.6 | 13.6   | 31.2   | 20      | 1.2 |
| <a href="#">Lab028</a> | 2                               | 13.2                         | 13.1         | 14         | 0.7 | 5.3    | 11.4   | 20      | 3.6 | 13.2           | 13.7                        | 296        | 1.2 | 8.8    | 21.3   | 20      | 1.8 |
| <a href="#">Lab031</a> | 2                               | 12.8                         | -            | 0          | -   | -      | -      | 20      | -   | 12.8           | 10.4                        | 89         | 1.5 | 14.4   | 47.6   | 20      | 0.1 |
| <a href="#">Lab032</a> | 2                               | 12.3                         | -            | 0          | -   | -      | -      | 20      | -   | 12.3           | 11.5                        | 222        | 1.9 | 16.5   | 39.5   | 20      | 0.8 |
| <a href="#">Lab033</a> | 2                               | 11.5                         | 11.8         | 5          | 0.5 | 4.2    | 11.1   | 20      | 4.1 | 11.5           | 12.0                        | 125        | 1.0 | 8.3    | 21.0   | 20      | 1.9 |
| <a href="#">Lab034</a> | 2                               | 12.8                         | 12.0         | 5          | 1.1 | 9.2    | 24.6   | 20      | 1.5 | 12.8           | 12.4                        | 73         | 0.7 | 5.6    | 14.4   | 20      | 3.0 |
| <a href="#">Lab035</a> | 2                               | 12.8                         | -            | 0          | -   | -      | -      | 20      | -   | 12.8           | 12.4                        | 55         | 0.7 | 5.6    | 14.4   | 20      | 3.0 |
| <a href="#">Lab037</a> | 2                               | 12.6                         | 12.9         | 5          | 1.1 | 8.5    | 19.4   | 20      | 2.1 | 12.6           | 12.7                        | 40         | 1.2 | 9.4    | 19.7   | 20      | 2.0 |
| <a href="#">Lab038</a> | 2                               | 12.8                         | -            | 0          | -   | -      | -      | 20      | -   | 12.8           | 12.7                        | 55         | 1.0 | 7.9    | 16.5   | 20      | 2.4 |
| <a href="#">Lab040</a> | 2                               | 12.8                         | 12.0         | 6          | 0.5 | 4.2    | 14.6   | 20      | 3.3 | 12.8           | 11.8                        | 11         | 0.5 | 4.2    | 16.3   | 20      | 2.9 |
| <b>Total</b>           | -                               | -                            | 12.2         | 50         | 1.1 | 9.0    | -      | -       | -   | -              | 12.1                        | 1793       | 1.7 | 14.0   | -      | -       | -   |

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month :

Cumulative : from    to

[TOP](#)

### Control D Month vs. Cumulative

|                        |                                 | Control D (Lot No.: AC1203D) |              |            |     |        |        |         |     |                |                             |            |     |        |        |         |     |
|------------------------|---------------------------------|------------------------------|--------------|------------|-----|--------|--------|---------|-----|----------------|-----------------------------|------------|-----|--------|--------|---------|-----|
|                        |                                 | Month (2016/09)              |              |            |     |        |        |         |     |                | CUM (2014/02/01~2016/09/30) |            |     |        |        |         |     |
| UnitID <sup>⬇</sup>    | Reagent Kit (Code) <sup>⬇</sup> | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   | Target (U/gHb) | Mean (U/gHb)                | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   |
| <a href="#">Lab017</a> | 2                               | 3.3                          | -            | 0          | -   | -      | -      | 20      | -   | 3.3            | 3.9                         | 36         | 1.4 | 35.9   | 90.0   | 20      | 0.1 |
| <a href="#">Lab018</a> | 2                               | 2.7                          | 2.3          | 4          | 0.3 | 13.0   | 40.9   | 20      | 0.4 | 2.7            | 2.6                         | 105        | 0.9 | 34.6   | 72.9   | 20      | 0.5 |
| <a href="#">Lab019</a> | 2                               | 2.9                          | 3.0          | 4          | 0.1 | 3.3    | 10.1   | 20      | 5.0 | 2.9            | 2.8                         | 136        | 0.4 | 14.3   | 32.0   | 20      | 1.2 |
| <a href="#">Lab021</a> | 2                               | 2.9                          | 2.9          | 5          | 0.2 | 6.9    | 13.8   | 20      | 2.9 | 2.9            | 3.3                         | 76         | 0.3 | 9.1    | 32.0   | 20      | 0.7 |
| <a href="#">Lab022</a> | 2                               | 3.3                          | 2.8          | 2          | -   | -      | -      | 20      | -   | 3.3            | 2.9                         | 57         | 0.3 | 10.3   | 32.8   | 20      | 0.8 |
| <a href="#">Lab024</a> | 2                               | 2.7                          | -            | 0          | -   | -      | -      | 20      | -   | 2.7            | 2.7                         | 58         | 0.3 | 11.1   | 22.2   | 20      | 1.8 |
| <a href="#">Lab026</a> | 2                               | 2.7                          | -            | 0          | -   | -      | -      | 36      | -   | 2.7            | 2.8                         | 212        | 0.5 | 17.9   | 39.4   | 36      | 1.8 |
| <a href="#">Lab027</a> | 2                               | 2.9                          | -            | 0          | -   | -      | -      | 20      | -   | 2.9            | 2.7                         | 147        | 0.5 | 18.5   | 43.9   | 20      | 0.7 |
| <a href="#">Lab028</a> | 2                               | 3.2                          | 3.2          | 14         | 0.3 | 9.4    | 18.8   | 20      | 2.1 | 3.2            | 3.3                         | 296        | 0.5 | 15.2   | 33.4   | 20      | 1.1 |
| <a href="#">Lab031</a> | 2                               | 2.9                          | -            | 0          | -   | -      | -      | 20      | -   | 2.9            | 2.5                         | 89         | 0.5 | 20.0   | 53.8   | 20      | 0.3 |
| <a href="#">Lab032</a> | 2                               | 2.9                          | -            | 0          | -   | -      | -      | 20      | -   | 2.9            | 2.7                         | 222        | 0.5 | 18.5   | 43.9   | 20      | 0.7 |
| <a href="#">Lab033</a> | 2                               | 2.7                          | 2.9          | 5          | 0.2 | 6.9    | 21.2   | 20      | 1.8 | 2.7            | 2.9                         | 125        | 0.3 | 10.3   | 28.1   | 20      | 1.2 |
| <a href="#">Lab034</a> | 2                               | 2.9                          | 2.8          | 5          | 0.4 | 14.3   | 32.0   | 20      | 1.2 | 2.9            | 3.0                         | 73         | 0.2 | 6.7    | 16.8   | 20      | 2.5 |
| <a href="#">Lab035</a> | 2                               | 2.9                          | -            | 0          | -   | -      | -      | 20      | -   | 2.9            | 2.8                         | 55         | 0.3 | 10.7   | 24.9   | 20      | 1.5 |
| <a href="#">Lab037</a> | 2                               | 3.0                          | 3.1          | 5          | 0.4 | 12.9   | 29.1   | 20      | 1.3 | 3.0            | 3.0                         | 40         | 0.4 | 13.3   | 26.7   | 20      | 1.5 |
| <a href="#">Lab038</a> | 2                               | 2.9                          | -            | 0          | -   | -      | -      | 20      | -   | 2.9            | 3.1                         | 55         | 0.5 | 16.1   | 39.2   | 20      | 0.8 |
| <a href="#">Lab040</a> | 2                               | 2.9                          | 2.3          | 6          | 0.4 | 17.4   | 55.5   | 20      | 0.0 | 2.9            | 2.4                         | 11         | 0.3 | 12.5   | 42.2   | 20      | 0.2 |
| <b>Total</b>           | -                               | -                            | 2.9          | 50         | 0.4 | 13.8   | -      | -       | -   | -              | 2.9                         | 1793       | 0.6 | 20.7   | -      | -       | -   |

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month :

Cumulative : from    to

[TOP](#)

| Reagent Kit | Reagent Code |
|-------------|--------------|
| AMP         | 2            |