

QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) [Change](#)

[Print Table](#)

Lab022

	Control N		Control D	
QC Control Lot No.	AH1220N		AH1220D	
Duration of the Analyzing	Month (2019/08)	CUM (2019/02/01~2019/08/31)	Month (2019/08)	CUM (2019/02/01~2019/08/31)
Runs (N)	5	17	5	17
Mean (U/gHb)	12.2	12.4	4.0	4.0
SD	0.2	0.3	0.1	0.1
CV (%)	1.6	2.4	2.5	2.5
Target Value (U/gHb)	12.4	12.4	4.1	4.1
Total Error (%)	4.9	4.8	7.4	7.4
TEa (%)	20	20	20	20
σ	>6	>6	>6	>6

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 x CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)


Month : 2019 08 [Change](#) ; Cumulative : from 2019 02 01 to 2019 08 31 [Change](#)

[TOP](#)

Control N SDI QC Chart

Lot No.: AH1220N ; Duration : 2019-02-01 to 2019-08-31 ; Target : 12.4 ; SD : 0.8

Lab022

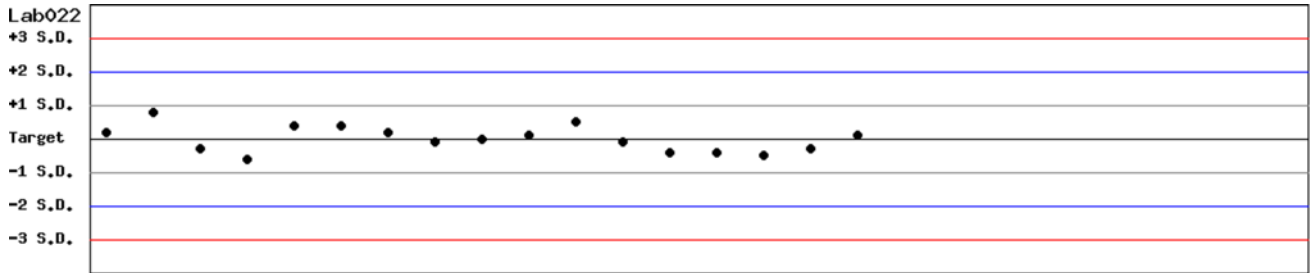

Date 05-03 05-10 05-18 05-24 06-01 06-11 06-14 07-04 07-12 07-18 07-19 07-25 08-01 08-08 08-08 08-21 08-29


Month : 2019 08 [Change](#) ; Cumulative : from 2019 02 01 to 2019 08 31 [Change](#)

[TOP](#)

Control D SDI QC Chart

Lot No.: AH1220D ; Duration : 2019-02-01 to 2019-08-31 ; Target : 4.1 ; SD : 0.4

Lab022

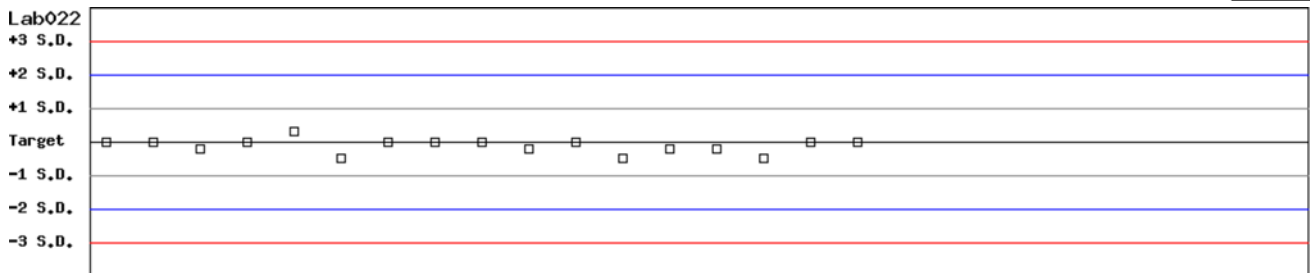

Date 05-03 05-10 05-18 05-24 06-01 06-11 06-14 07-04 07-12 07-18 07-19 07-25 08-01 08-08 08-08 08-21 08-29

Month : 2019 08 [Change](#) ; Cumulative : from 2019 02 01 to 2019 08 31 [Change](#)


[TOP](#)

Control N and Control D SDI QC Chart

Lot No.: AH1220N ; Duration : 2019-02-01 to 2019-08-31 ; Target : 12.4 ; SD : 0.8 (●)

Lot No.: AH1220D ; Duration : 2019-02-01 to 2019-08-31 ; Target : 4.1 ; SD : 0.4 (□)

Lab022

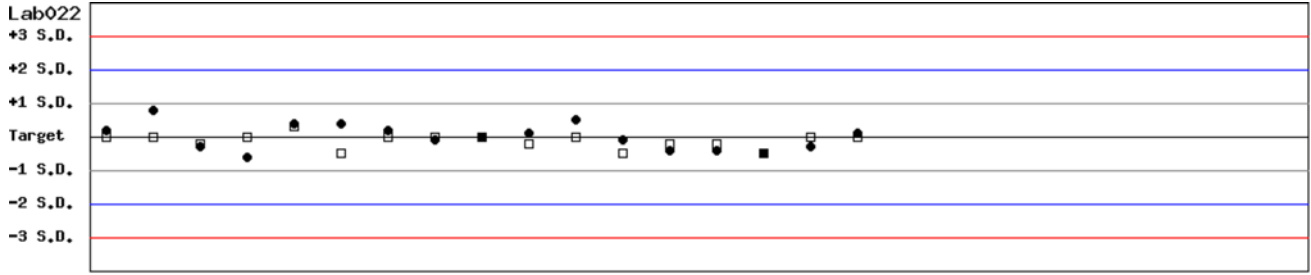

Date 05-03 05-10 05-18 05-24 06-01 06-11 06-14 07-04 07-12 07-18 07-19 07-25 08-01 08-08 08-08 08-21 08-29

Month : 2019 08 ; Cumulative : from 2019 02 01 to 2019 08 31

[\[TOP\]](#)

Peer Group Statistics (Table 1)

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31)

Select Reagent Kit : 5 - Medicon

Monthly

Month : 2019 08

		Control N (Lot No.: AH1220N)								Control D (Lot No.: AH1220D)							
UnitID <input type="button" value="↑"/>	Reagent Kit (Code) <input type="button" value="↑"/>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab020	5	15.9	15.1	4	0.5	3.3	11.7	20	4.5	5.2	4.8	4	0.2	4.2	16.0	20	2.9
Lab022	5	12.4	12.2	5	0.2	1.6	4.9	20	>6	4.1	4.0	5	0.1	2.5	7.4	20	>6
Lab032	5	15.3	14.5	6	0.5	3.4	12.1	20	4.3	5.2	4.4	6	0.2	4.5	24.5	20	1.0
Lab033	5	12.4	12.8	5	0.3	2.3	7.9	20	>6	3.9	3.8	5	0.2	5.3	13.1	20	3.3
Total	-	-	13.6	20	1.2	8.8	-	-	-	-	4.2	20	0.4	9.5	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[\[TOP\]](#)

Cumulative

Cumulative : from 2019 02 01 to 2019 08 31

		Control N (Lot No.: AH1220N)								Control D (Lot No.: AH1220D)							
UnitID <input type="button" value="↑"/>	Reagent Kit (Code) <input type="button" value="↑"/>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab020	5	15.9	15.2	10	0.6	3.9	12.3	20	4.0	5.2	4.6	10	0.2	4.3	20.2	20	2.0
Lab022	5	12.4	12.4	17	0.3	2.4	4.8	20	>6	4.1	4.0	17	0.1	2.5	7.4	20	>6
Lab032	5	15.3	14.3	19	0.6	4.2	14.9	20	3.2	5.2	4.6	19	0.6	13.0	37.6	20	0.7
Lab033	5	12.4	12.5	21	0.4	3.2	7.2	20	6.0	3.9	3.9	21	0.1	2.6	5.1	20	>6
Total	-	-	13.4	67	1.2	9.0	-	-	-	-	4.2	67	0.5	11.9	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[\[TOP\]](#)

Reagent Kit	Reagent Code
Medicon	5

Peer Group Statistics (Table 2)

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 5 - Medicon ▼ Change

Print Table 2

Control N Month vs. Cumulative

		Control N (Lot No.: AH1220N)															
		Month (2019/08)								CUM (2019/02/01~2019/08/31)							
UnitID ↑	Reagent Kit (Code) ↑	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab020	5	15.9	15.1	4	0.5	3.3	11.7	20	4.5	15.9	15.2	10	0.6	3.9	12.3	20	4.0
Lab022	5	12.4	12.2	5	0.2	1.6	4.9	20	>6	12.4	12.4	17	0.3	2.4	4.8	20	>6
Lab032	5	15.3	14.5	6	0.5	3.4	12.1	20	4.3	15.3	14.3	19	0.6	4.2	14.9	20	3.2
Lab033	5	12.4	12.8	5	0.3	2.3	7.9	20	>6	12.4	12.5	21	0.4	3.2	7.2	20	6.0
Total	-	-	13.6	20	1.2	8.8	-	-	-	-	13.4	67	1.2	9.0	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2019 ▼ 08 ▼ Change Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2019 ▼ 08 ▼ 31 ▼ Change

[TOP](#)

Control D Month vs. Cumulative

		Control D (Lot No.: AH1220D)															
		Month (2019/08)								CUM (2019/02/01~2019/08/31)							
UnitID ↑	Reagent Kit (Code) ↑	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab020	5	5.2	4.8	4	0.2	4.2	16.0	20	2.9	5.2	4.6	10	0.2	4.3	20.2	20	2.0
Lab022	5	4.1	4.0	5	0.1	2.5	7.4	20	>6	4.1	4.0	17	0.1	2.5	7.4	20	>6
Lab032	5	5.2	4.4	6	0.2	4.5	24.5	20	1.0	5.2	4.6	19	0.6	13.0	37.6	20	0.7
Lab033	5	3.9	3.8	5	0.2	5.3	13.1	20	3.3	3.9	3.9	21	0.1	2.6	5.1	20	>6
Total	-	-	4.2	20	0.4	9.5	-	-	-	-	4.2	67	0.5	11.9	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month : 2019 ▼ 08 ▼ Change Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2019 ▼ 08 ▼ 31 ▼ Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5