

# QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) [Change](#)

[Print Table](#)

## Lab022

QC Control Lot No.	Control N		Control D	
	AH1220N		AH1220D	
Duration of the Analyzing	Month (2019/10)	CUM (2019/02/01~2019/10/31)	Month (2019/10)	CUM (2019/02/01~2019/10/31)
Runs (N)	7	25	7	25
Mean (U/gHb)	12.3	12.4	4.1	4.1
SD	0.3	0.3	0.1	0.1
CV (%)	2.4	2.4	2.4	2.4
Target Value (U/gHb)	12.4	12.4	4.1	4.1
Total Error (%)	5.7	4.8	4.9	4.9
TEa (%)	20	20	20	20
$\sigma$	>6	>6	>6	>6

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 x CV (%)

$\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)


Month : 2019 | 10 | [Change](#) ; Cumulative : from 2019 | 02 | 01 to 2019 | 10 | 31 | [Change](#)

[\[TOP\]](#)

## Control N SDI QC Chart

Lot No.: AH1220N ; Duration : 2019-02-01 to 2019-10-31 ; Target : 12.4 ; SD : 0.8

Lab022

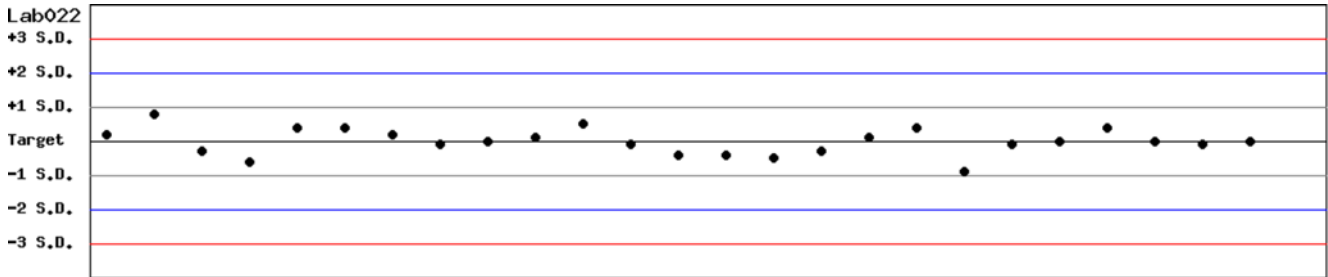

Date 05-03 05-10 05-18 05-24 06-01 06-11 06-14 07-04 07-12 07-18 07-19 07-25 08-01 08-08 08-08 08-21 08-29 09-05 10-02 10-03 10-10 10-15 10-21 10-23 10-31

Month : 2019 | 10 | [Change](#) ; Cumulative : from 2019 | 02 | 01 to 2019 | 10 | 31 | [Change](#)

[\[TOP\]](#)

## Control D SDI QC Chart

Lot No.: AH1220D ; Duration : 2019-02-01 to 2019-10-31 ; Target : 4.1 ; SD : 0.4

Lab022



Date 05-03 05-10 05-18 05-24 06-01 06-11 06-14 07-04 07-12 07-18 07-19 07-25 08-01 08-08 08-08 08-21 08-29 09-05 10-02 10-03 10-10 10-15 10-21 10-23 10-31

Month : 2019 | 10 | [Change](#) ; Cumulative : from 2019 | 02 | 01 to 2019 | 10 | 31 | [Change](#)


[\[TOP\]](#)

## Control N and Control D SDI QC Chart

Lot No.: AH1220N ; Duration : 2019-02-01 to 2019-10-31 ; Target : 12.4 ; SD : 0.8 (●)

Lot No.: AH1220D ; Duration : 2019-02-01 to 2019-10-31 ; Target : 4.1 ; SD : 0.4 (□)

Lab022

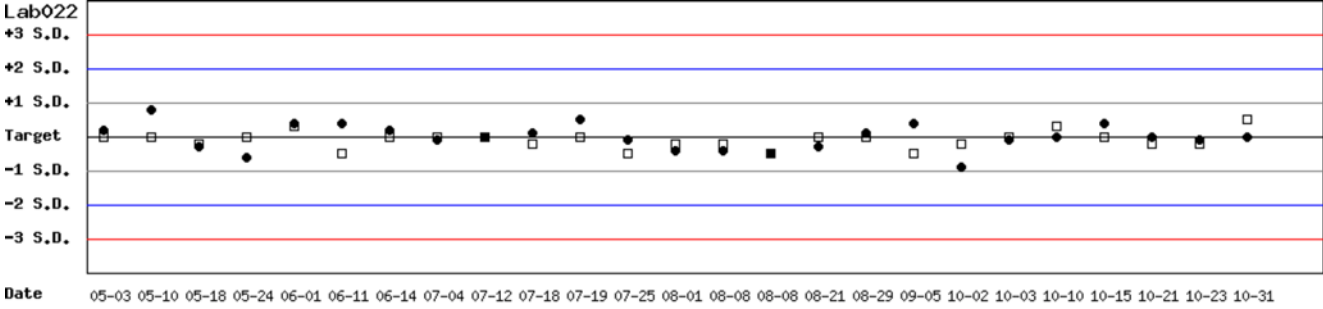

Month : 2019 | 10 |  ; Cumulative : from 2019 | 02 | 01 to 2019 | 10 | 31 |

[\[TOP\]](#)

# Peer Group Statistics (Table 1)

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 5 - Medicon ▼ Change

Print Table 1

## Monthly

Month : 2019 ▼ 10 ▼ Change

		Control N (Lot No.: AH1220N)								Control D (Lot No.: AH1220D)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	15.9	15.9	3	0.8	5.0	10.1	20	4.0	5.2	5.1	3	0.1	2.0	5.8	20	>6
<a href="#">Lab022</a>	5	12.4	12.3	7	0.3	2.4	5.7	20	>6	4.1	4.1	7	0.1	2.4	4.9	20	>6
<a href="#">Lab032</a>	5	15.3	14.9	3	0.2	1.3	5.3	20	>6	5.2	4.8	3	0.7	14.6	36.9	20	0.8
<a href="#">Lab033</a>	5	12.4	12.8	5	0.3	2.3	7.9	20	>6	3.9	3.8	5	0.1	2.6	7.8	20	>6
<b>Total</b>	-	-	13.5	18	1.5	11.1	-	-	-	-	4.3	18	0.5	11.6	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

## Cumulative

Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2019 ▼ 10 ▼ 31 ▼ Change

		Control N (Lot No.: AH1220N)								Control D (Lot No.: AH1220D)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	15.9	15.3	16	0.6	3.9	11.6	20	4.2	5.2	4.7	16	0.2	4.3	18.1	20	2.4
<a href="#">Lab022</a>	5	12.4	12.4	25	0.3	2.4	4.8	20	>6	4.1	4.1	25	0.1	2.4	4.9	20	>6
<a href="#">Lab032</a>	5	15.3	14.5	29	0.5	3.4	12.1	20	4.3	5.2	4.6	29	0.5	10.9	33.3	20	0.8
<a href="#">Lab033</a>	5	12.4	12.6	30	0.4	3.2	8.0	20	5.7	3.9	3.9	30	0.1	2.6	5.1	20	>6
<b>Total</b>	-	-	13.5	100	1.3	9.6	-	-	-	-	4.3	100	0.5	11.6	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

Reagent Kit	Reagent Code
Medicon	5

## Peer Group Statistics (Table 2)

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 5 - Medicon ▼ Change

Print Table 2

### Control N Month vs. Cumulative

		Control N (Lot No.: AH1220N)															
		Month (2019/10)								CUM (2019/02/01~2019/10/31)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	15.9	15.9	3	0.8	5.0	10.1	20	4.0	15.9	15.3	16	0.6	3.9	11.6	20	4.2
<a href="#">Lab022</a>	5	12.4	12.3	7	0.3	2.4	5.7	20	>6	12.4	12.4	25	0.3	2.4	4.8	20	>6
<a href="#">Lab032</a>	5	15.3	14.9	3	0.2	1.3	5.3	20	>6	15.3	14.5	29	0.5	3.4	12.1	20	4.3
<a href="#">Lab033</a>	5	12.4	12.8	5	0.3	2.3	7.9	20	>6	12.4	12.6	30	0.4	3.2	8.0	20	5.7
Total	-	-	13.5	18	1.5	11.1	-	-	-	-	13.5	100	1.3	9.6	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2019 ▼ 10 ▼ Change Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2019 ▼ 10 ▼ 31 ▼ Change

[TOP](#)

### Control D Month vs. Cumulative

		Control D (Lot No.: AH1220D)															
		Month (2019/10)								CUM (2019/02/01~2019/10/31)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	5.2	5.1	3	0.1	2.0	5.8	20	>6	5.2	4.7	16	0.2	4.3	18.1	20	2.4
<a href="#">Lab022</a>	5	4.1	4.1	7	0.1	2.4	4.9	20	>6	4.1	4.1	25	0.1	2.4	4.9	20	>6
<a href="#">Lab032</a>	5	5.2	4.8	3	0.7	14.6	36.9	20	0.8	5.2	4.6	29	0.5	10.9	33.3	20	0.8
<a href="#">Lab033</a>	5	3.9	3.8	5	0.1	2.6	7.8	20	>6	3.9	3.9	30	0.1	2.6	5.1	20	>6
Total	-	-	4.3	18	0.5	11.6	-	-	-	-	4.3	100	0.5	11.6	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2019 ▼ 10 ▼ Change Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2019 ▼ 10 ▼ 31 ▼ Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5