

# QC Chart of Internal Quality Control (IQC)for G6PD Quantitative Test

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) [Change](#)

[Print Table](#)

## Lab020

	Control N		Control D	
QC Control Lot No.	AH1220N		AH1220D	
Duration of the Analyzing	Month (2020/05)	CUM (2019/06/18~2020/05/30)	Month (2020/05)	CUM (2019/06/18~2020/05/30)
Runs (N)	1	17	1	17
Mean (U/gHb)	13.3	15.2	4.4	4.7
SD	-	0.8	-	0.2
CV (%)	-	5.3	-	4.3
Target Value (U/gHb)	15.9	15.9	5.2	5.2
Total Error (%)	-	14.9	-	18.1
TEa (%)	20	20	20	20
$\sigma$	-	2.9	-	2.4

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

$\sigma$  (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2020 05 [Change](#) ; Cumulative : from 2019 06 18 to 2020 05 30 [Change](#)


[TOP](#)

## Control N and Control D SDI QC Chart

Lot No.: AH1220N ; Duration : 2019-06-18 to 2020-05-30 ; Target : 15.9 ; SD : 0.70 ( ● )

Lot No.: AH1220D ; Duration : 2019-06-18 to 2020-05-30 ; Target : 5.2 ; SD : 0.40 ( □ )

Lab020

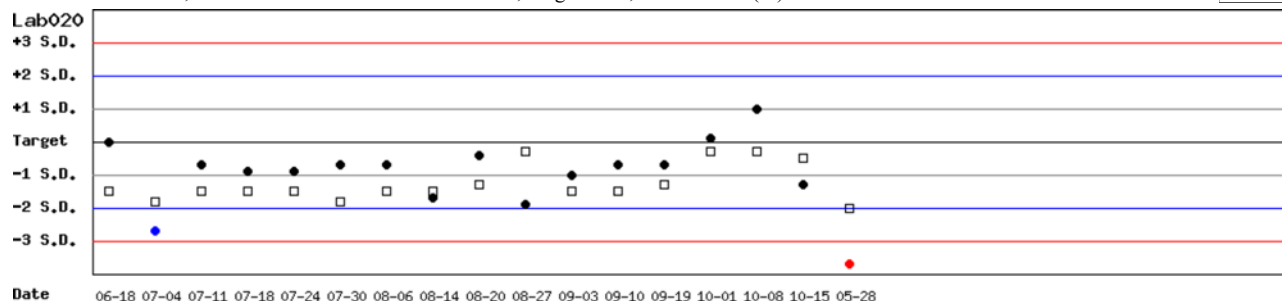


Month : 2020 05 [Change](#) ; Cumulative : from 2019 06 18 to 2020 05 30 [Change](#)

[TOP](#)

## Control N SDI QC Chart

Lot No.: AH1220N ; Duration : 2019-06-18 to 2020-05-30 ; Target : 15.9 ; SD : 0.70

Lab020

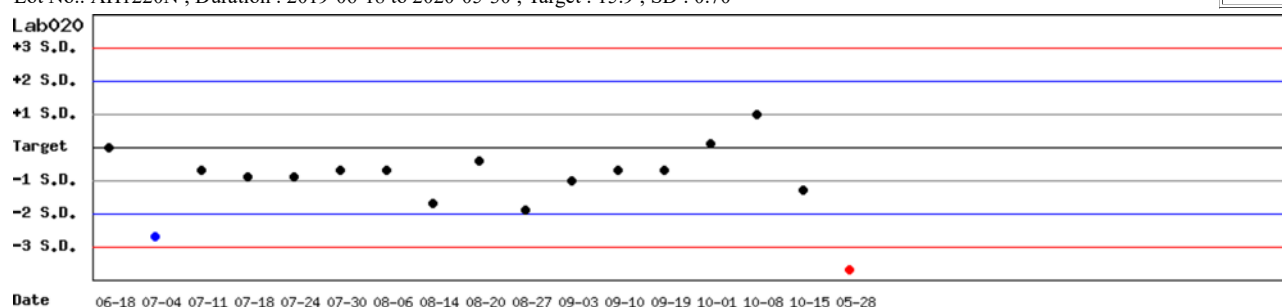


Month : 2020 05 [Change](#) ; Cumulative : from 2019 06 18 to 2020 05 30 [Change](#)

[TOP](#)

## Control D SDI QC Chart

Lot No.: AH1220D ; Duration : 2019-06-18 to 2020-05-30 ; Target : 5.2 ; SD : 0.40

Lab020

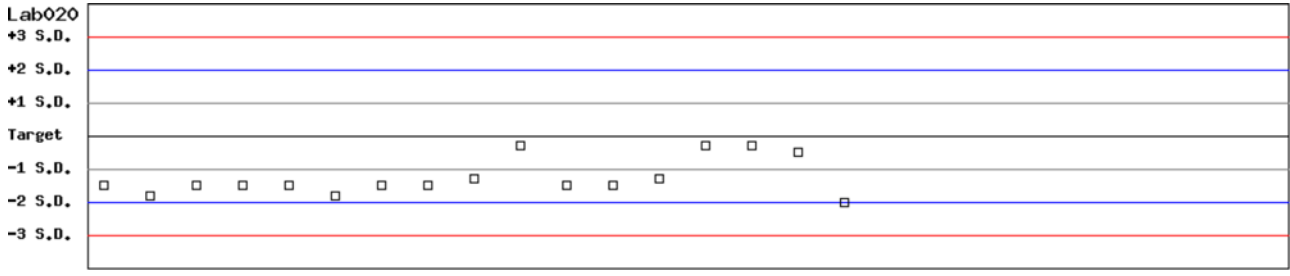

Date 06-18 07-04 07-11 07-18 07-24 07-30 08-06 08-14 08-20 08-27 09-03 09-10 09-19 10-01 10-08 10-15 05-28

Month : 2020 05  ; Cumulative : from 2019 06 18 to 2020 05 30

[TOP](#)

# Peer Group Statistics (Table 1)

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 5 - Medicon ▼ Change

Print Table 1

## Monthly

Month : 2020 ▼ 05 ▼ Change

		Control N (Lot No.: AH1220N)								Control D (Lot No.: AH1220D)							
UnitID <span style="font-size: small;">↑</span>	Reagent Kit (Code) <span style="font-size: small;">↑</span>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	15.9	13.3	1	-	-	-	20	-	5.2	4.4	1	-	-	-	20	-
<a href="#">Lab032</a>	5	15.3	13.0	6	0.5	3.8	22.7	20	1.3	5.2	4.0	6	0.1	2.5	28.1	20	1.2
<a href="#">Lab033</a>	5	12.4	12.3	3	0.2	1.6	4.1	20	>6	3.9	3.9	3	0.1	2.6	5.1	20	>6
<a href="#">Lab037</a>	5	15.3	15.2	3	0.2	1.3	3.3	20	>6	5.2	4.7	3	0.2	4.3	18.1	20	2.4
<b>Total</b>	-	-	13.4	13	1.1	8.2	-	-	-	-	4.2	13	0.3	7.1	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

## Cumulative

Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2020 ▼ 05 ▼ 31 ▼ Change

		Control N (Lot No.: AH1220N)								Control D (Lot No.: AH1220D)							
UnitID <span style="font-size: small;">↑</span>	Reagent Kit (Code) <span style="font-size: small;">↑</span>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	15.9	15.2	17	0.8	5.3	14.9	20	2.9	5.2	4.7	17	0.2	4.3	18.1	20	2.4
<a href="#">Lab022</a>	5	12.4	12.3	41	0.4	3.3	7.3	20	5.8	4.1	4.0	41	0.1	2.5	7.4	20	>6
<a href="#">Lab032</a>	5	15.3	14.2	68	0.6	4.2	15.6	20	3.1	5.2	4.4	68	0.4	9.1	33.6	20	0.5
<a href="#">Lab033</a>	5	12.4	12.5	56	0.4	3.2	7.2	20	6.0	3.9	3.9	56	0.1	2.6	5.1	20	>6
<a href="#">Lab037</a>	5	15.3	15.3	16	0.4	2.6	5.2	20	>6	5.2	4.7	16	0.2	4.3	18.1	20	2.4
<b>Total</b>	-	-	13.5	198	1.2	8.9	-	-	-	-	4.2	198	0.4	9.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[TOP](#)

<b>Reagent Kit</b>	<b>Reagent Code</b>
Medicon	5

## Peer Group Statistics (Table 2)

Select LotNo : AH1220N (2019-01-28 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 5 - Medicon ▼ Change

[Print Table 2](#)

### Control N Month vs. Cumulative

		Control N (Lot No.: AH1220N)															
		Month (2020/05)								CUM (2019/02/01~2020/05/31)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	15.9	13.3	1	-	-	-	20	-	15.9	15.2	17	0.8	5.3	14.9	20	2.9
<a href="#">Lab022</a>	5	12.4	-	0	-	-	-	20	-	12.4	12.3	41	0.4	3.3	7.3	20	5.8
<a href="#">Lab032</a>	5	15.3	13.0	6	0.5	3.8	22.7	20	1.3	15.3	14.2	68	0.6	4.2	15.6	20	3.1
<a href="#">Lab033</a>	5	12.4	12.3	3	0.2	1.6	4.1	20	>6	12.4	12.5	56	0.4	3.2	7.2	20	6.0
<a href="#">Lab037</a>	5	15.3	15.2	3	0.2	1.3	3.3	20	>6	15.3	15.3	16	0.4	2.6	5.2	20	>6
<b>Total</b>	-	-	13.4	13	1.1	8.2	-	-	-	-	13.5	198	1.2	8.9	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2020 ▼ 05 ▼ Change Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2020 ▼ 05 ▼ 31 ▼ Change

[TOP](#)

### Control D Month vs. Cumulative

		Control D (Lot No.: AH1220D)															
		Month (2020/05)								CUM (2019/02/01~2020/05/31)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab020</a>	5	5.2	4.4	1	-	-	-	20	-	5.2	4.7	17	0.2	4.3	18.1	20	2.4
<a href="#">Lab022</a>	5	4.1	-	0	-	-	-	20	-	4.1	4.0	41	0.1	2.5	7.4	20	>6
<a href="#">Lab032</a>	5	5.2	4.0	6	0.1	2.5	28.1	20	-1.2	5.2	4.4	68	0.4	9.1	33.6	20	0.5
<a href="#">Lab033</a>	5	3.9	3.9	3	0.1	2.6	5.1	20	>6	3.9	3.9	56	0.1	2.6	5.1	20	>6
<a href="#">Lab037</a>	5	5.2	4.7	3	0.2	4.3	18.1	20	2.4	5.2	4.7	16	0.2	4.3	18.1	20	2.4
<b>Total</b>	-	-	4.2	13	0.3	7.1	-	-	-	-	4.2	198	0.4	9.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2020 ▼ 05 ▼ Change Cumulative : from 2019 ▼ 02 ▼ 01 ▼ to 2020 ▼ 05 ▼ 31 ▼ Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5