

# G6PD 定量檢驗內部品管統計結果及 SDI 分佈圖

選擇 LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) Change

列印圖表

檢驗單位 : **Lab006**

| QC Control Lot No. | Control N       |                             | Control D       |                             |
|--------------------|-----------------|-----------------------------|-----------------|-----------------------------|
|                    | BJ0922N         |                             | BJ0922D         |                             |
| 檢驗期間               | Month (2022/12) | CUM (2022/07/15~2022/12/31) | Month (2022/12) | CUM (2022/07/15~2022/12/31) |
| 累計點數 (N)           | 4               | 26                          | 4               | 26                          |
| 累計平均值 (Mean) U/gHb | 15.5            | 15.5                        | 5.1             | 5.3                         |
| 累計標準差 (SD)         | 0.2             | 0.4                         | 0.1             | 0.2                         |
| 累計變異係數 (CV) %      | 1.3             | 2.6                         | 2.0             | 3.8                         |
| 目標值 (Target) U/gHb | 15.6            | 15.6                        | 5.3             | 5.3                         |
| 總誤差 (TE) %         | 3.2             | 5.8                         | 7.7             | 7.5                         |
| 可容許總誤差 (TEa) %     | 20              | 20                          | 20              | 20                          |
| $\sigma$           | >6              | >6                          | >6              | 5.3                         |

誤差 (Bias)% =  $\{ [ | \text{累計平均值 (Mean)} - \text{目標值 (Target)} | ] / \text{目標值 (Target)} \} \times 100\%$   
 總誤差 (TE, Total Error)% = 誤差 (Bias)% + 2 × 累計變異係數 (CV)  
 $\sigma$  (Sigma) = (TEa% - 誤差 (Bias)% ) / 累計變異係數 (CV)

月統計 : 2022 12 Change ; 累計期間 (CUM) : 自 2022 07 15 至 2022 12 31 Change


[\[TOP\]](#)

## Control N 及 Control D SDI 分佈圖

Lot No.: BJ0922N; 檢驗期間 : 2022-07-15 至 2022-12-31; 目標值 (Target) : 15.6; 參考標準差 (SD) : 1.00 (●)

Lot No.: BJ0922D; 檢驗期間 : 2022-07-15 至 2022-12-31; 目標值 (Target) : 5.3; 參考標準差 (SD) : 0.20 (□)

單位 : Lab006

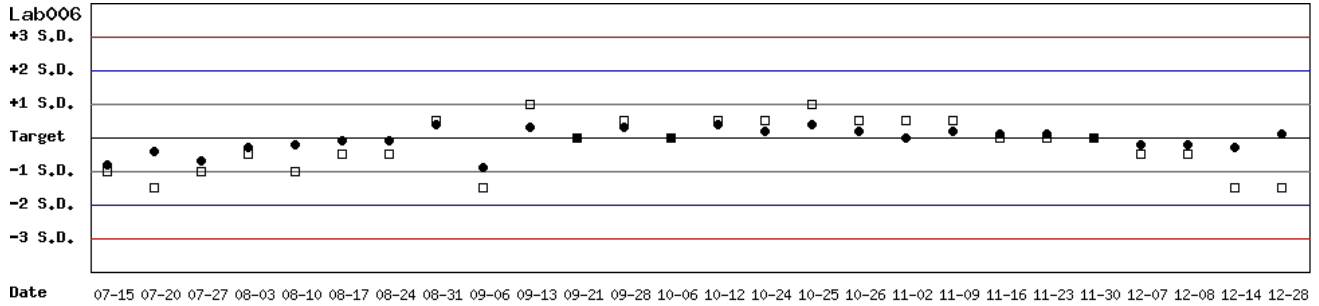


月統計 : 2022 12 Change ; 累計期間 (CUM) : 自 2022 07 15 至 2022 12 31 Change

[\[TOP\]](#)

## Control N SDI 分佈圖

Lot No.: BJ0922N; 檢驗期間 : 2022-07-15 至 2022-12-31; 目標值 (Target) : 15.6; 參考標準差 (SD) : 1.00

單位 : Lab006

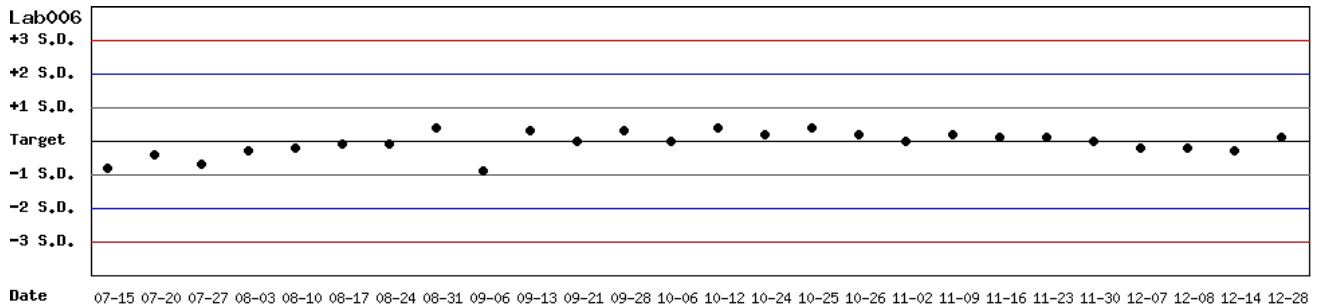


月統計 : 2022 12 Change ; 累計期間 (CUM) : 自 2022 07 15 至 2022 12 31 Change

[\[TOP\]](#)

# Control D SDI 分佈圖

Lot No.: BJ0922D; 檢驗期間: 2022-07-15 至 2022-12-31; 目標值 (Target): 5.3; 參考標準差 (SD): 0.20

單位: Lab006

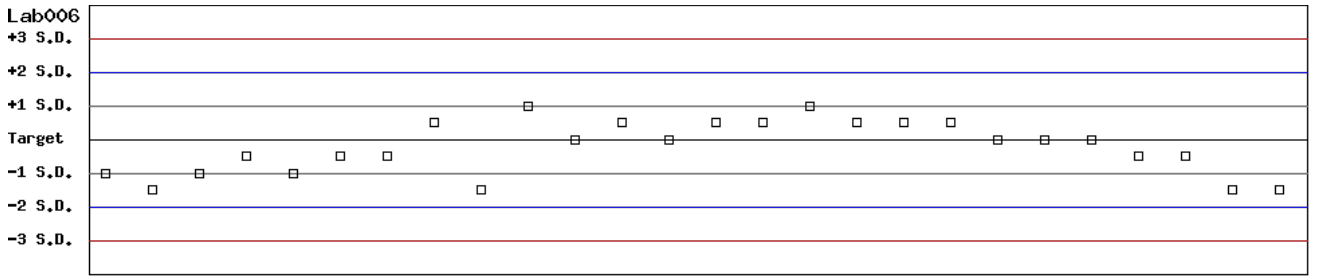

Date 07-15 07-20 07-27 08-03 08-10 08-17 08-24 08-31 09-06 09-13 09-21 09-28 10-06 10-12 10-24 10-25 10-26 11-02 11-09 11-16 11-23 11-30 12-07 12-08 12-14 12-28

月統計: 2022 12 Change ; 累計期間 (CUM): 自 2022 07 15 至 2022 12 31 Change

[TOP](#)

# 各檢驗單位 G6PD 定量檢驗 內部品管統計結果 (總表一)

選擇 LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) Change

選擇 Reagent Kit : 4 - Lanner Change

[列印總表一](#)

## 月統計表

統計月份 : 2022 12 Change

| UnitID <span>↑</span>  | Reagent Kit (Code) <span>↑</span> | Control N (Lot No.: BJ0922N) |              |            |     |        |        |         |          |                | Control D (Lot No.: BJ0922D) |            |     |        |        |         |          |
|------------------------|-----------------------------------|------------------------------|--------------|------------|-----|--------|--------|---------|----------|----------------|------------------------------|------------|-----|--------|--------|---------|----------|
|                        |                                   | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | $\sigma$ | Target (U/gHb) | Mean (U/gHb)                 | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | $\sigma$ |
| <a href="#">Lab006</a> | 4                                 | 15.6                         | 15.5         | 4          | 0.2 | 1.3    | 3.2    | 20      | >6       | 5.3            | 5.1                          | 4          | 0.1 | 2.0    | 7.7    | 20      | >6       |
| <a href="#">Lab008</a> | 4                                 | 16.0                         | 15.9         | 9          | 0.2 | 1.3    | 3.1    | 20      | >6       | 5.6            | 5.4                          | 9          | 0.2 | 3.7    | 11.0   | 20      | 4.4      |
| <a href="#">Lab010</a> | 4                                 | 16.7                         | 16.7         | 1          | -   | -      | -      | 20      | -        | 5.8            | 5.6                          | 1          | -   | -      | -      | 20      | -        |
| <a href="#">Lab011</a> | 4                                 | 15.8                         | 15.4         | 5          | 0.2 | 1.3    | 5.1    | 20      | >6       | 5.2            | 5.1                          | 5          | 0.2 | 3.9    | 9.8    | 20      | 4.6      |
| Total                  | -                                 | -                            | 15.7         | 19         | 0.4 | 2.5    | -      | -       | -        | -              | 5.3                          | 19         | 0.2 | 3.8    | -      | -       | -        |

誤差 (Bias)% =  $\{ [ | \text{累計平均值 (Mean)} - \text{目標值 (Target)} | ] / \text{目標值 (Target)} \} \times 100\%$

總誤差 (TE, Total Error)% = 誤差 (Bias)% + 2 × 累計變異係數 (CV)

$\sigma$  (Sigma) = (TEa% - 誤差 (Bias)%) / 累計變異係數 (CV)

[TOP](#)

## 累計統計表

累計期間 : 自 2021 01 01 至 2022 12 31 Change

| UnitID <span>↑</span>  | Reagent Kit (Code) <span>↑</span> | Control N (Lot No.: BJ0922N) |              |            |     |        |        |         |          |                | Control D (Lot No.: BJ0922D) |            |     |        |        |         |          |
|------------------------|-----------------------------------|------------------------------|--------------|------------|-----|--------|--------|---------|----------|----------------|------------------------------|------------|-----|--------|--------|---------|----------|
|                        |                                   | Target (U/gHb)               | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | $\sigma$ | Target (U/gHb) | Mean (U/gHb)                 | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | $\sigma$ |
| <a href="#">Lab006</a> | 4                                 | 15.6                         | 15.5         | 77         | 0.6 | 3.9    | 8.4    | 20      | 5.0      | 5.3            | 5.3                          | 77         | 0.2 | 3.8    | 7.5    | 20      | 5.3      |
| <a href="#">Lab007</a> | 4                                 | 16.7                         | 16.9         | 154        | 1.1 | 6.5    | 14.2   | 20      | 2.9      | 5.3            | 5.7                          | 154        | 0.3 | 5.3    | 18.1   | 20      | 2.3      |
| <a href="#">Lab008</a> | 4                                 | 16.0                         | 14.8         | 98         | 0.9 | 6.1    | 19.7   | 20      | 2.0      | 5.6            | 5.0                          | 98         | 0.3 | 6.0    | 22.7   | 20      | 1.5      |
| <a href="#">Lab009</a> | 4                                 | 16.3                         | 15.6         | 96         | 0.8 | 5.1    | 14.6   | 20      | 3.1      | 5.9            | 5.3                          | 96         | 0.3 | 5.7    | 21.5   | 20      | 1.7      |
| <a href="#">Lab010</a> | 4                                 | 16.7                         | 15.9         | 32         | 0.6 | 3.8    | 12.3   | 20      | 4.0      | 5.8            | 5.5                          | 32         | 0.2 | 3.6    | 12.4   | 20      | 4.1      |
| <a href="#">Lab011</a> | 4                                 | 15.8                         | 16.2         | 56         | 0.8 | 4.9    | 12.4   | 20      | 3.6      | 5.2            | 5.4                          | 56         | 0.4 | 7.4    | 18.7   | 20      | 2.2      |
| <a href="#">Lab012</a> | 4                                 | 15.7                         | 15.6         | 151        | 0.8 | 5.1    | 10.9   | 20      | 3.8      | 5.3            | 5.4                          | 151        | 0.3 | 5.6    | 13.0   | 20      | 3.2      |
| Total                  | -                                 | -                            | 15.8         | 664        | 1.1 | 7.0    | -      | -       | -        | -              | 5.4                          | 664        | 0.4 | 7.4    | -      | -       | -        |

誤差 (Bias)% =  $\{ [ | \text{累計平均值 (Mean)} - \text{目標值 (Target)} | ] / \text{目標值 (Target)} \} \times 100\%$

總誤差 (TE, Total Error)% = 誤差 (Bias)% + 2 × 累計變異係數 (CV)

$\sigma$  (Sigma) = (TEa% - 誤差 (Bias)%) / 累計變異係數 (CV)

[TOP](#)

| Reagent Kit | Reagent Code |
|-------------|--------------|
| Lanner      | 4            |

各檢驗單位 G6PD 定量檢驗 內部品管統計結果 (總表二)

選擇 LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) Change

選擇 Reagent Kit : 4 - Lanner Change

列印總表二

Control N 月統計與累計統計之比較表

| Control N (Lot No.: BJ0922N) |                      |                 |              |            |     |        |        |         |    |                |                             |            |     |        |        |         |     |
|------------------------------|----------------------|-----------------|--------------|------------|-----|--------|--------|---------|----|----------------|-----------------------------|------------|-----|--------|--------|---------|-----|
|                              |                      | Month (2022/12) |              |            |     |        |        |         |    |                | CUM (2021/01/01~2022/12/31) |            |     |        |        |         |     |
| UnitID ↑                     | Reagent Kit (Code) ↑ | Target (U/gHb)  | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ  | Target (U/gHb) | Mean (U/gHb)                | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   |
| <a href="#">Lab006</a>       | 4                    | 15.6            | 15.5         | 4          | 0.2 | 1.3    | 3.2    | 20      | >6 | 15.6           | 15.5                        | 77         | 0.6 | 3.9    | 8.4    | 20      | 5.0 |
| <a href="#">Lab007</a>       | 4                    | 16.7            | -            | 0          | -   | -      | -      | 20      | -  | 16.7           | 16.9                        | 154        | 1.1 | 6.5    | 14.2   | 20      | 2.9 |
| <a href="#">Lab008</a>       | 4                    | 16.0            | 15.9         | 9          | 0.2 | 1.3    | 3.1    | 20      | >6 | 16.0           | 14.8                        | 98         | 0.9 | 6.1    | 19.7   | 20      | 2.0 |
| <a href="#">Lab009</a>       | 4                    | 16.3            | -            | 0          | -   | -      | -      | 20      | -  | 16.3           | 15.6                        | 96         | 0.8 | 5.1    | 14.6   | 20      | 3.1 |
| <a href="#">Lab010</a>       | 4                    | 16.7            | 16.7         | 1          | -   | -      | -      | 20      | -  | 16.7           | 15.9                        | 32         | 0.6 | 3.8    | 12.3   | 20      | 4.0 |
| <a href="#">Lab011</a>       | 4                    | 15.8            | 15.4         | 5          | 0.2 | 1.3    | 5.1    | 20      | >6 | 15.8           | 16.2                        | 56         | 0.8 | 4.9    | 12.4   | 20      | 3.6 |
| <a href="#">Lab012</a>       | 4                    | 15.7            | -            | 0          | -   | -      | -      | 20      | -  | 15.7           | 15.6                        | 151        | 0.8 | 5.1    | 10.9   | 20      | 3.8 |
| Total                        | -                    | -               | 15.7         | 19         | 0.4 | 2.5    | -      | -       | -  | -              | 15.8                        | 664        | 1.1 | 7.0    | -      | -       | -   |

誤差 (Bias)% = { [ | 累計平均值 (Mean) - 目標值 (Target) | ] / 目標值 (Target) } x 100%

總誤差 (TE, Total Error)% = 誤差 (Bias)% + 2 x 累計變異係數 (CV)

σ (Sigma) = (TEa% - 誤差 (Bias)% ) / 累計變異係數 (CV)

月統計 : 2022 12 Change

累計期間 (CUM) : 自 2021 01 01 至 2022 12 31 Change

[TOP](#)

Control D 月統計與累計統計之比較表

| Control D (Lot No.: BJ0922D) |                      |                 |              |            |     |        |        |         |     |                |                             |            |     |        |        |         |     |
|------------------------------|----------------------|-----------------|--------------|------------|-----|--------|--------|---------|-----|----------------|-----------------------------|------------|-----|--------|--------|---------|-----|
|                              |                      | Month (2022/12) |              |            |     |        |        |         |     |                | CUM (2021/01/01~2022/12/31) |            |     |        |        |         |     |
| UnitID ↑                     | Reagent Kit (Code) ↑ | Target (U/gHb)  | Mean (U/gHb) | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   | Target (U/gHb) | Mean (U/gHb)                | n for Mean | SD  | CV (%) | TE (%) | TEa (%) | σ   |
| <a href="#">Lab006</a>       | 4                    | 5.3             | 5.1          | 4          | 0.1 | 2.0    | 7.7    | 20      | >6  | 5.3            | 5.3                         | 77         | 0.2 | 3.8    | 7.5    | 20      | 5.3 |
| <a href="#">Lab007</a>       | 4                    | 5.3             | -            | 0          | -   | -      | -      | 20      | -   | 5.3            | 5.7                         | 154        | 0.3 | 5.3    | 18.1   | 20      | 2.3 |
| <a href="#">Lab008</a>       | 4                    | 5.6             | 5.4          | 9          | 0.2 | 3.7    | 11.0   | 20      | 4.4 | 5.6            | 5.0                         | 98         | 0.3 | 6.0    | 22.7   | 20      | 1.5 |
| <a href="#">Lab009</a>       | 4                    | 5.9             | -            | 0          | -   | -      | -      | 20      | -   | 5.9            | 5.3                         | 96         | 0.3 | 5.7    | 21.5   | 20      | 1.7 |
| <a href="#">Lab010</a>       | 4                    | 5.8             | 5.6          | 1          | -   | -      | -      | 20      | -   | 5.8            | 5.5                         | 32         | 0.2 | 3.6    | 12.4   | 20      | 4.1 |
| <a href="#">Lab011</a>       | 4                    | 5.2             | 5.1          | 5          | 0.2 | 3.9    | 9.8    | 20      | 4.6 | 5.2            | 5.4                         | 56         | 0.4 | 7.4    | 18.7   | 20      | 2.2 |
| <a href="#">Lab012</a>       | 4                    | 5.3             | -            | 0          | -   | -      | -      | 20      | -   | 5.3            | 5.4                         | 151        | 0.3 | 5.6    | 13.0   | 20      | 3.2 |
| Total                        | -                    | -               | 5.3          | 19         | 0.2 | 3.8    | -      | -       | -   | -              | 5.4                         | 664        | 0.4 | 7.4    | -      | -       | -   |

誤差 (Bias)% = { [ | 累計平均值 (Mean) - 目標值 (Target) | ] / 目標值 (Target) } x 100%

總誤差 (TE, Total Error)% = 誤差 (Bias)% + 2 x 累計變異係數 (CV)

σ (Sigma) = (TEa% - 誤差 (Bias)% ) / 累計變異係數 (CV)

月統計 : 2022 12 Change

累計期間 (CUM) : 自 2021 01 01 至 2022 12 31 Change

[TOP](#)

| Reagent Kit | Reagent Code |
|-------------|--------------|
| Lanner      | 4            |