

# Summary Report of IQC program for G6PD Quantitative Test - Medicon Group - December 2022 -


## I. The statistic results of all laboratories in this month

G6PD	Control N (Lot No.:BJ0922N)	Control D (Lot No.: BJ0922D)
Labs	8	8
Received results number (n)	36	36
Median	14.4 (U/g Hb)	4.7 (U/g Hb)
Mean	14.3 (U/g Hb)	4.7 (U/g Hb)
SD	0.5	0.2
CV	3.5%	4.3%
Range of G6PD	13.4 ~ 15.7 (U/g Hb)	4.4 ~ 5.2 (U/g Hb)
Range of Hb	2.0 ~ 2.6 (g/dL)	1.8 ~ 2.3 (g/dL)

\*The statistic results are calculated from all labs reported in this month

\*\* G6PD Method = Medicon reagent kit, 37°C

## II. The distribution of G6PD reported for each lab in this survey

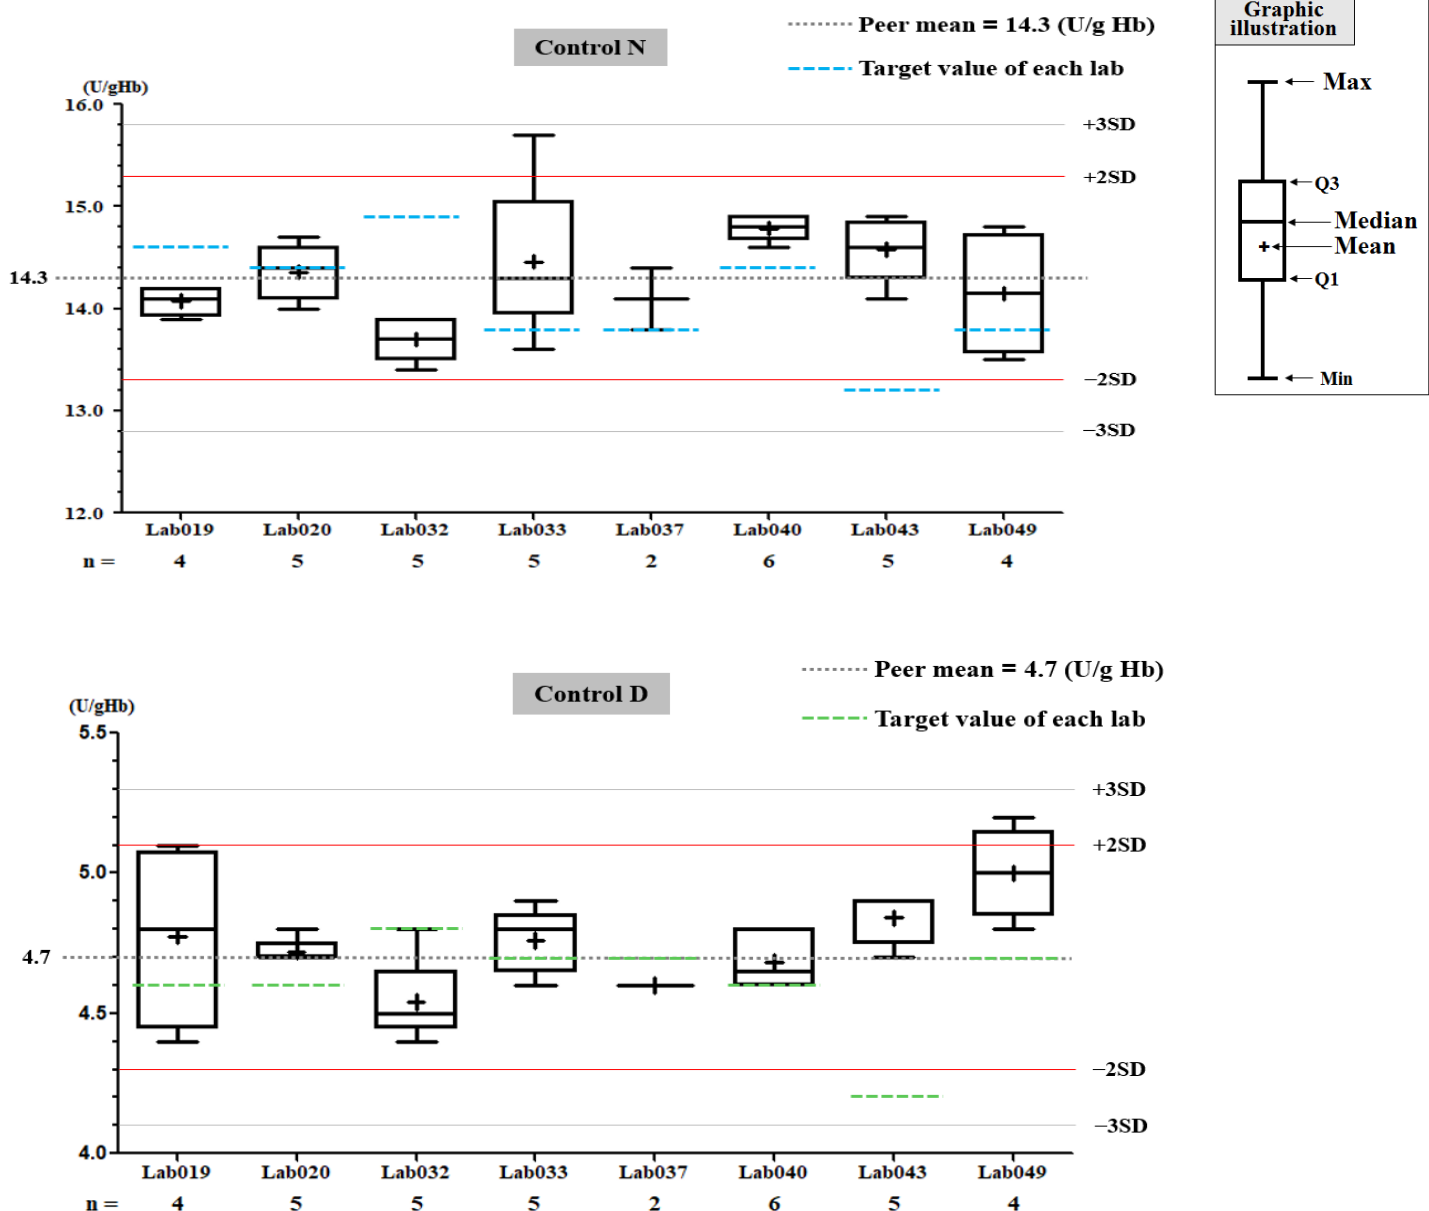

# QC Chart of Internal Quality Control (IQC) for G6PD Quantitative Test

Select LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) ▾ Change

Print Table

## Lab033

QC Control Lot No.	Control N		Control D	
	BJ0922N		BJ0922D	
Duration of the Analyzing	Month (2022/12)	CUM (2022/06/30~2022/12/31)	Month (2022/12)	CUM (2022/06/30~2022/12/31)
Runs (N)	5	26	5	26
Mean (U/gHb)	14.5	13.9	4.8	4.7
SD	0.8	0.5	0.1	0.1
CV (%)	5.5	3.6	2.1	2.1
Target Value (U/gHb)	13.8	13.8	4.7	4.7
Total Error (%)	16.1	7.9	6.3	4.3
TEa (%)	20	20	20	20
σ	2.7	5.4	>6	>6

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%  
 TE : Total Error(%) = Bias (%) + 2 x CV (%)  
 σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2022 ▾ 12 ▾ Change ; Cumulative : from 2022 ▾ 06 ▾ 30 ▾ to 2022 ▾ 12 ▾ 31 ▾ Change


[\[TOP\]](#)

## Control N and Control D SDI QC Chart

Lot No.: BJ0922N ; Duration : 2022-06-30 to 2022-12-31 ; Target : 13.8 ; SD : 1.38 ( ● )

Lot No.: BJ0922D ; Duration : 2022-06-30 to 2022-12-31 ; Target : 4.7 ; SD : 0.47 ( □ )

Lab033

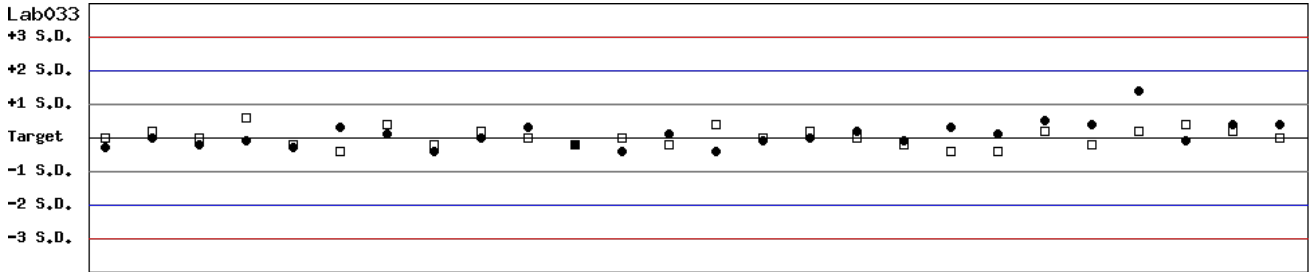

Date 06-30 07-07 07-14 07-21 07-28 08-04 08-18 08-25 09-01 09-08 09-15 09-22 09-29 10-06 10-13 10-20 10-27 11-03 11-10 11-17 11-24 12-01 12-08 12-15 12-22 12-29


Month : 2022 ▾ 12 ▾ Change ; Cumulative : from 2022 ▾ 06 ▾ 30 ▾ to 2022 ▾ 12 ▾ 31 ▾ Change

[\[TOP\]](#)

## Control N SDI QC Chart

Lot No.: BJ0922N ; Duration : 2022-06-30 to 2022-12-31 ; Target : 13.8 ; SD : 1.38

Lab033

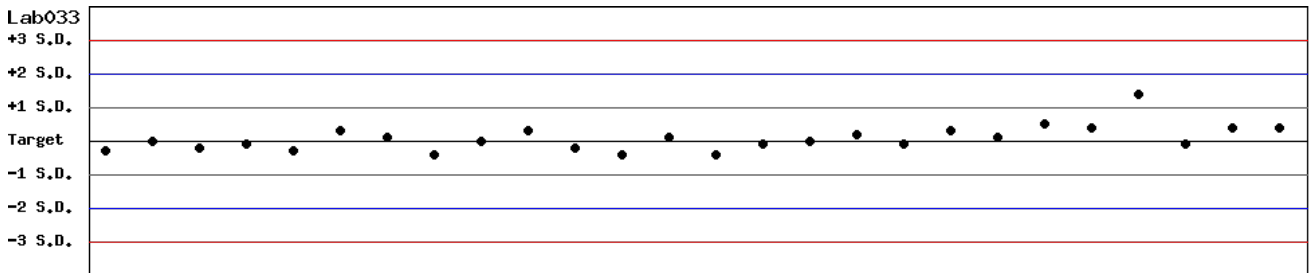

Date 06-30 07-07 07-14 07-21 07-28 08-04 08-18 08-25 09-01 09-08 09-15 09-22 09-29 10-06 10-13 10-20 10-27 11-03 11-10 11-17 11-24 12-01 12-08 12-15 12-22 12-29


Month : 2022 ▾ 12 ▾ Change ; Cumulative : from 2022 ▾ 06 ▾ 30 ▾ to 2022 ▾ 12 ▾ 31 ▾ Change

[\[TOP\]](#)

# Control D SDI QC Chart

Lab033

Lot No.: BJ0922D ; Duration : 2022-06-30 to 2022-12-31 ; Target : 4.7 ; SD : 0.47

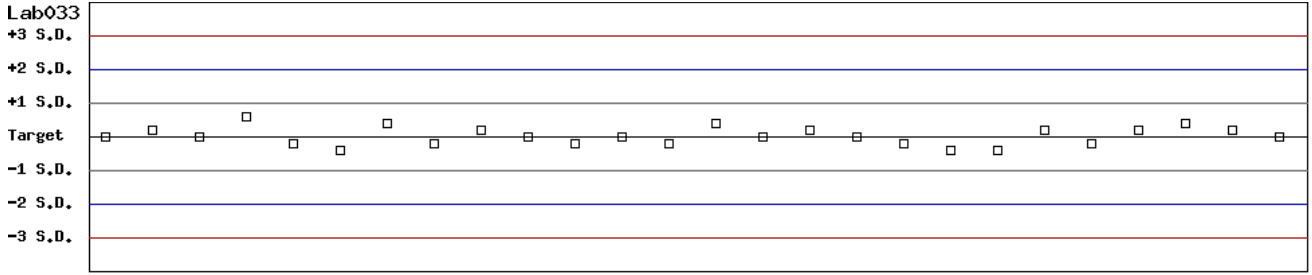

Date 06-30 07-07 07-14 07-21 07-28 08-04 08-18 08-25 09-01 09-08 09-15 09-22 09-29 10-06 10-13 10-20 10-27 11-03 11-10 11-17 11-24 12-01 12-08 12-15 12-22 12-29

Month : 2022 v 12 v Change ; Cumulative : from 2022 v 06 v 30 v to 2022 v 12 v 31 v Change

[TOP](#)

## Peer Group Statistics (Table 1)

Select LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

Print Table 1

### Monthly

Month : 2022 12 Change

UnitID <small>↑</small>	Reagent Kit (Code) <small>↑</small>	Control N (Lot No.: BJ0922N)									Control D (Lot No.: BJ0922D)						
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab019</a>	5	14.6	14.1	4	0.2	1.4	6.3	20	>6	4.6	4.8	4	0.3	6.3	16.8	20	2.5
<a href="#">Lab020</a>	5	14.4	14.4	5	0.3	2.1	4.2	20	>6	4.6	4.7	5	0.0	0.0	2.2	20	>6
<a href="#">Lab032</a>	5	14.9	13.7	5	0.2	1.5	11.0	20	>6	4.8	4.5	5	0.2	4.4	15.1	20	3.1
<a href="#">Lab033</a>	5	13.8	14.5	5	0.8	5.5	16.1	20	2.7	4.7	4.8	5	0.1	2.1	6.3	20	>6
<a href="#">Lab037</a>	5	13.8	14.1	2	-	-	-	20	-	4.7	4.6	2	-	-	-	20	-
<a href="#">Lab040</a>	5	14.4	14.8	6	0.1	0.7	4.1	20	>6	4.6	4.7	6	0.1	2.1	6.4	20	>6
<a href="#">Lab043</a>	5	13.2	14.6	5	0.3	2.1	14.7	20	4.5	4.2	4.8	5	0.1	2.1	18.5	20	2.7
<a href="#">Lab049</a>	5	13.8	14.2	4	0.6	4.2	11.3	20	4.1	4.7	5.0	4	0.2	4.0	14.4	20	3.4
Total	-	-	14.3	36	0.5	3.5	-	-	-	-	4.7	36	0.2	4.3	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

### Cumulative

Cumulative : from 2021 01 01 to 2022 12 31 Change

UnitID <small>↑</small>	Reagent Kit (Code) <small>↑</small>	Control N (Lot No.: BJ0922N)									Control D (Lot No.: BJ0922D)						
		Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	16.2	16.4	8	0.4	2.4	6.1	20	>6	5.5	5.5	8	0.2	3.6	7.3	20	5.6
<a href="#">Lab019</a>	5	14.6	14.3	40	0.6	4.2	10.4	20	4.3	4.6	4.6	40	0.2	4.3	8.7	20	4.7
<a href="#">Lab020</a>	5	14.4	14.4	51	0.6	4.2	8.3	20	4.8	4.6	4.7	51	0.1	2.1	6.4	20	>6
<a href="#">Lab022</a>	5	14.4	14.3	17	0.5	3.5	7.7	20	5.5	4.6	4.5	17	0.2	4.4	11.1	20	4.1
<a href="#">Lab028</a>	5	15.2	15.1	34	1.1	7.3	15.2	20	2.6	4.9	4.9	34	0.3	6.1	12.2	20	3.3
<a href="#">Lab032</a>	5	14.9	14.4	106	0.4	2.8	8.9	20	5.9	4.8	4.5	106	0.1	2.2	10.7	20	>6
<a href="#">Lab033</a>	5	13.8	13.6	51	0.6	4.4	10.3	20	4.2	4.7	4.6	51	0.3	6.5	15.2	20	2.7
<a href="#">Lab037</a>	5	13.8	14.6	46	0.4	2.7	11.3	20	5.3	4.7	4.7	46	0.2	4.3	8.5	20	4.7
<a href="#">Lab040</a>	5	14.4	14.6	31	0.2	1.4	4.1	20	>6	4.6	4.6	31	0.1	2.2	4.3	20	>6
<a href="#">Lab043</a>	5	13.2	13.6	69	1.4	10.3	23.6	20	1.6	4.2	4.4	69	0.5	11.4	27.5	20	1.3
<a href="#">Lab049</a>	5	13.8	14.6	81	0.7	4.8	15.4	20	3.0	4.7	4.7	81	0.2	4.3	8.5	20	4.7
Total	-	-	14.3	534	0.9	6.3	-	-	-	-	4.6	534	0.3	6.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

[\[TOP\]](#)

Reagent Kit	Reagent Code
Medicon	5

## Peer Group Statistics (Table 2)

Select LotNo : BJ0922N (2021-01-01 ~ 2100-12-31) ▼ Change

Select Reagent Kit : 5 - Medicon ▼ Change

[Print Table 2](#)

### Control N Month vs. Cumulative

		Control N (Lot No.: BJ0922N)															
		Month (2022/12)								CUM (2021/01/01~2022/12/31)							
UnitID <small>↑</small>	Reagent Kit (Code) <small>↑</small>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	16.2	-	0	-	-	-	20	-	16.2	16.4	8	0.4	2.4	6.1	20	>6
<a href="#">Lab019</a>	5	14.6	14.1	4	0.2	1.4	6.3	20	>6	14.6	14.3	40	0.6	4.2	10.4	20	4.3
<a href="#">Lab020</a>	5	14.4	14.4	5	0.3	2.1	4.2	20	>6	14.4	14.4	51	0.6	4.2	8.3	20	4.8
<a href="#">Lab022</a>	5	14.4	-	0	-	-	-	20	-	14.4	14.3	17	0.5	3.5	7.7	20	5.5
<a href="#">Lab028</a>	5	15.2	-	0	-	-	-	20	-	15.2	15.1	34	1.1	7.3	15.2	20	2.6
<a href="#">Lab032</a>	5	14.9	13.7	5	0.2	1.5	11.0	20	>6	14.9	14.4	106	0.4	2.8	8.9	20	5.9
<a href="#">Lab033</a>	5	13.8	14.5	5	0.8	5.5	16.1	20	2.7	13.8	13.6	51	0.6	4.4	10.3	20	4.2
<a href="#">Lab037</a>	5	13.8	14.1	2	-	-	-	20	-	13.8	14.6	46	0.4	2.7	11.3	20	5.3
<a href="#">Lab040</a>	5	14.4	14.8	6	0.1	0.7	4.1	20	>6	14.4	14.6	31	0.2	1.4	4.1	20	>6
<a href="#">Lab043</a>	5	13.2	14.6	5	0.3	2.1	14.7	20	4.5	13.2	13.6	69	1.4	10.3	23.6	20	1.6
<a href="#">Lab049</a>	5	13.8	14.2	4	0.6	4.2	11.3	20	4.1	13.8	14.6	81	0.7	4.8	15.4	20	3.0
Total	-	-	14.3	36	0.5	3.5	-	-	-	-	14.3	534	0.9	6.3	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2022 ▼ 12 ▼ Change

Cumulative : from 2021 ▼ 01 ▼ 01 ▼ to 2022 ▼ 12 ▼ 31 ▼ Change

[TOP](#)

### Control D Month vs. Cumulative

		Control D (Lot No.: BJ0922D)															
		Month (2022/12)								CUM (2021/01/01~2022/12/31)							
UnitID <small>↑</small>	Reagent Kit (Code) <small>↑</small>	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
<a href="#">Lab018</a>	5	5.5	-	0	-	-	-	20	-	5.5	5.5	8	0.2	3.6	7.3	20	5.6
<a href="#">Lab019</a>	5	4.6	4.8	4	0.3	6.3	16.8	20	2.5	4.6	4.6	40	0.2	4.3	8.7	20	4.7
<a href="#">Lab020</a>	5	4.6	4.7	5	0.0	0.0	2.2	20	>6	4.6	4.7	51	0.1	2.1	6.4	20	>6
<a href="#">Lab022</a>	5	4.6	-	0	-	-	-	20	-	4.6	4.5	17	0.2	4.4	11.1	20	4.1
<a href="#">Lab028</a>	5	4.9	-	0	-	-	-	20	-	4.9	4.9	34	0.3	6.1	12.2	20	3.3
<a href="#">Lab032</a>	5	4.8	4.5	5	0.2	4.4	15.1	20	3.1	4.8	4.5	106	0.1	2.2	10.7	20	>6
<a href="#">Lab033</a>	5	4.7	4.8	5	0.1	2.1	6.3	20	>6	4.7	4.6	51	0.3	6.5	15.2	20	2.7
<a href="#">Lab037</a>	5	4.7	4.6	2	-	-	-	20	-	4.7	4.7	46	0.2	4.3	8.5	20	4.7
<a href="#">Lab040</a>	5	4.6	4.7	6	0.1	2.1	6.4	20	>6	4.6	4.6	31	0.1	2.2	4.3	20	>6
<a href="#">Lab043</a>	5	4.2	4.8	5	0.1	2.1	18.5	20	2.7	4.2	4.4	69	0.5	11.4	27.5	20	1.3
<a href="#">Lab049</a>	5	4.7	5.0	4	0.2	4.0	14.4	20	3.4	4.7	4.7	81	0.2	4.3	8.5	20	4.7
Total	-	-	4.7	36	0.2	4.3	-	-	-	-	4.6	534	0.3	6.5	-	-	-

Bias (%) = [ ( | Mean - Target | ) / Target ] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%) ] / CV (%)

Month : 2022 ▼ 12 ▼ Change

Cumulative : from 2021 ▼ 01 ▼ 01 ▼ to 2022 ▼ 12 ▼ 31 ▼ Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5