

G6PD 定量檢驗內部品管統計結果及 SDI 分佈圖

選擇 LotNo : BD0728N (2024-08-20 ~ 2100-12-31) Change

列印圖表

檢驗單位 : Lab033

QC Control Lot No.	Control N		Control D	
	BD0728N		BD0728D	
檢驗期間	Month (2025/04)	CUM (2025/03/20~2025/04/30)	Month (2025/04)	CUM (2025/03/20~2025/04/30)
累計點數 (N)	4	6	4	6
累計平均值 (Mean) U/gHb	14.9	14.9	4.7	4.7
累計標準差 (SD)	0.5	0.4	0.1	0.1
累計變異係數 (CV) %	3.4	2.7	2.1	2.1
目標值 (Target) U/gHb	15.1	15.1	4.6	4.6
總誤差 (TE) %	8.0	6.7	6.4	6.4
可容許總誤差 (TEa) %	20	20	20	20
σ	5.5	>6	>6	>6

誤差 (Bias)% = { [| 累計平均值 (Mean) - 目標值 (Target) |] / 目標值 (Target) } x 100%
總誤差 (TE, Total Error)% = 誤差 (Bias)% + 2 x 累計變異係數 (CV)
σ (Sigma) = (TEa% - 誤差 (Bias)%) / 累計變異係數 (CV)

月統計 : 2025 04 Change ; 累計期間 (CUM) : 自 2025 03 20 至 2025 04 30 Change

[\[TOP\]](#)

Control N 及 Control D SDI
分佈圖

Lot No.: BD0728N; 檢驗期間 : 2025-03-20 至 2025-04-30 ; 目標值 (Target) : 15.1 ; 參考標準差 (SD) : 0.71 (●)

Lot No.: BD0728D; 檢驗期間 : 2025-03-20 至 2025-04-30 ; 目標值 (Target) : 4.6 ; 參考標準差 (SD) : 0.33 (□)

單位 : Lab033




月統計 : 2025 04 Change ; 累計期間 (CUM) : 自 2025 03 20 至 2025 04 30 Change

[\[TOP\]](#)

Control N SDI 分佈圖

Lot No.: BD0728N; 檢驗期間 : 2025-03-20 至 2025-04-30 ; 目標值 (Target) : 15.1 ; 參考標準差 (SD) : 0.71


單位 : Lab033

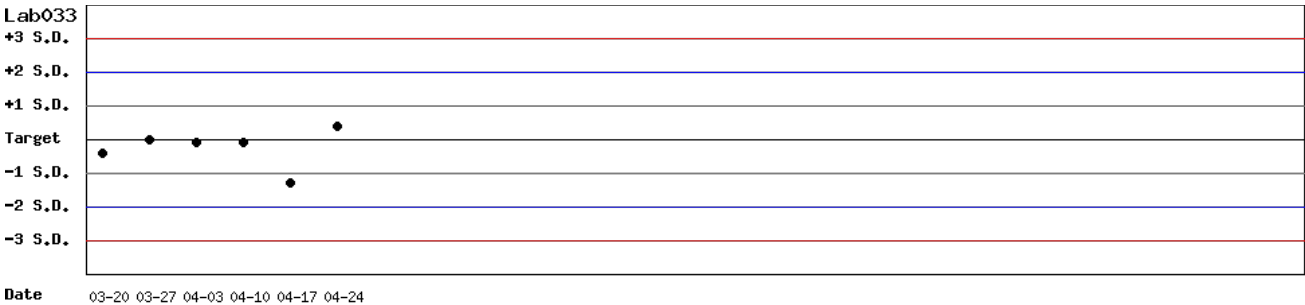

月統計 : 2025 04 Change ; 累計期間 (CUM) : 自 2025 03 20 至 2025 04 30 Change

[\[TOP\]](#)

Control D SDI 分佈圖

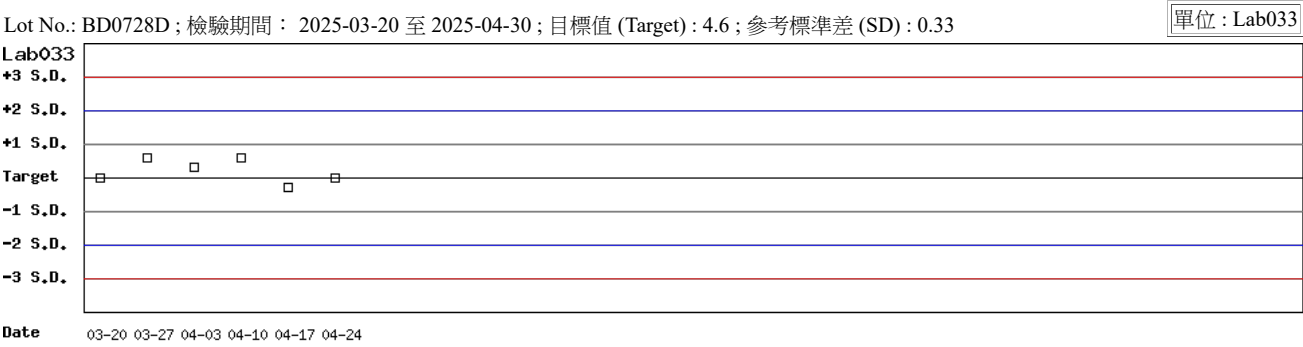

月統計：2025 04 Change ; 累計期間 (CUM)：自 2025 03 20 至 2025 04 30 Change

Peer Group Statistics (Table 1)

Select LotNo : BD0728N (2024-08-20 ~ 2100-12-31) Change

Select Reagent Kit : 5 - Medicon Change

Print Table 1

Monthly

Month : 2025 04 Change

		Control N (Lot No.: BD0728N)								Control D (Lot No.: BD0728D)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab033	5	14.1	14.9	4	0.5	3.4	12.4	20	4.2	4.1	4.7	4	0.1	2.1	18.9	20	2.6
Total	-	-	14.9	4	0.5	3.4	-	-	-	-	4.7	4	0.1	2.1	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE : Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[TOP]

Cumulative

Cumulative : from 2024 09 01 to 2025 04 30 Change

		Control N (Lot No.: BD0728N)								Control D (Lot No.: BD0728D)							
UnitID	Reagent Kit (Code)	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab033	5	14.1	14.9	6	0.4	2.7	11.0	20	5.3	4.1	4.7	6	0.1	2.1	18.9	20	2.6
Lab052	5	14.9	14.6	1	-	-	-	20	-	4.8	4.7	1	-	-	-	20	-
Total	-	-	14.9	7	0.4	2.7	-	-	-	-	4.7	7	0.1	2.1	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%
TE : Total Error(%) = Bias (%) + 2 × CV (%)
σ (Sigma) = [TEa% - Bias (%)] / CV (%)

[TOP]

Reagent Kit	Reagent Code
Medicon	5

Peer Group Statistics (Table 2)

Select LotNo :
BD0728N (2024-08-20 ~ 2100-12-31)
Change

Select Reagent Kit :
5 - Medicon
Change

Print Table 2

Control N Month vs.
Cumulative

Control N (Lot No.: BD0728N)																	
Month (2025/04)										CUM (2024/09/01~2025/04/30)							
UnitID 	Reagent Kit (Code) 	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab033	5	14.1	14.9	4	0.5	3.4	12.4	20	4.2	14.1	14.9	6	0.4	2.7	11.0	20	5.3
Lab052	5	14.9	-	0	-	-	-	20	-	14.9	14.6	1	-	-	-	20	-
Total	-	-	14.9	4	0.5	3.4	-	-	-	-	14.9	7	0.4	2.7	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month :
2025
04
Change
Cumulative : from
2024
09
01
to
2025
04
30
Change

[TOP](#)

Control D Month vs.
Cumulative

Control D (Lot No.: BD0728D)																	
Month (2025/04)										CUM (2024/09/01~2025/04/30)							
UnitID 	Reagent Kit (Code) 	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ	Target (U/gHb)	Mean (U/gHb)	n for Mean	SD	CV (%)	TE (%)	TEa (%)	σ
Lab033	5	4.1	4.7	4	0.1	2.1	18.9	20	2.6	4.1	4.7	6	0.1	2.1	18.9	20	2.6
Lab052	5	4.8	-	0	-	-	-	20	-	4.8	4.7	1	-	-	-	20	-
Total	-	-	4.7	4	0.1	2.1	-	-	-	-	4.7	7	0.1	2.1	-	-	-

Bias (%) = [(| Mean - Target |) / Target] x 100%

TE : Total Error(%) = Bias (%) + 2 × CV (%)

σ (Sigma) = [TEa% - Bias (%)] / CV (%)

Month :
2025
04
Change
Cumulative : from
2024
09
01
to
2025
04
30
Change

[TOP](#)

Reagent Kit	Reagent Code
Medicon	5