
Summary Report of IQC program for G6PD Quantitative Test - Medicon Group - May 2021 -


I. The statistic results of all laboratories in this month


G6PD	Control N (Lot No.:AH1220N)	Control D (Lot No.:AH1220D)
Labs	9	9
Received results number (n)	31	31
Median	14.2 (U/g Hb)	4.4 (U/g Hb)
Mean	14.0 (U/g Hb)	4.4 (U/g Hb)
SD	1.0	0.2
CV	7.1%	4.5%
Range of G6PD	$11.8 \sim 15.6 \; (U/g \; Hb)$	$3.8 \sim 4.8 \; (U/g \; Hb)$
Range of Hb	$2.0 \sim 2.5 \; (g/dL)$	$2.0 \sim 3.0 \; (g/dL)$

^{*}The statistic results are calculated from all labs reported in this month

II. The distribution of G6PD reported for each lab in this survey

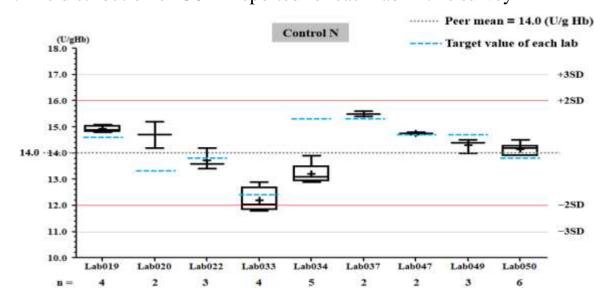



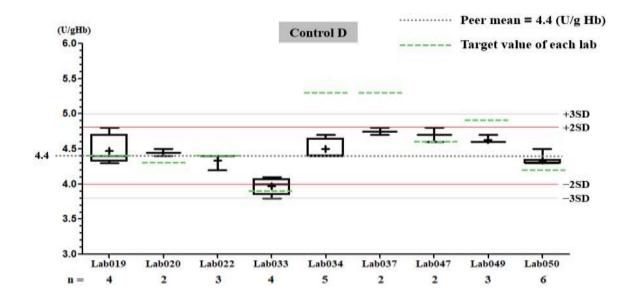



^{**} G6PD Method = Medicon reagent kit, 37°C